



## Sample gas cooler

### Series TC-MIDI X2

# Installation and Operation Instructions

Original instructions





Bühler Technologies GmbH, Harkortstr. 29, D-40880 Ratingen  
Tel. +49 (0) 21 02 / 49 89-0, Fax: +49 (0) 21 02 / 49 89-20  
Internet: [www.buehler-technologies.com](http://www.buehler-technologies.com)  
E-Mail: [analyse@buehler-technologies.com](mailto:analyse@buehler-technologies.com)

Read this instruction carefully prior to installation and/or use. Pay attention particularly to all advises and safety instructions to prevent injuries. Bühler Technologies can not be held responsible for misusing the product or unreliable function due to unauthorised modifications.

All rights reserved. Bühler Technologies GmbH 2025

Document information

Document No..... BE440024  
Version..... 10/2024

# Contents

1	Introduction .....	3
1.1	Intended use .....	3
1.2	Overview .....	4
1.3	Type plate .....	4
1.4	Scope of delivery .....	4
1.5	Ordering instructions.....	5
1.5.1	Gas cooler models with one gas path inside the heat exchanger .....	5
1.5.2	Gas cooler models with two gas paths inside the heat exchanger .....	6
1.5.3	Gas cooler models with one or two gas paths in the heat exchanger for H <sub>2</sub> /O <sub>2</sub> applications .....	7
1.5.4	Gas cooler models with two heat exchangers .....	8
1.5.5	Gas cooler models with two heat exchangers in series .....	9
2	Safety instructions .....	10
2.1	Important notices.....	10
2.2	General hazard warnings .....	11
3	Transport and storage .....	13
4	Installation and connection .....	14
4.1	Installation site requirements .....	14
4.2	Installation .....	14
4.2.1	Connecting the filter gas connections (optional) .....	15
4.2.2	Flow adapter connection (optional) .....	15
4.2.3	Connecting the moisture detector (option) .....	15
4.2.4	Sample gas pump connection gas lines (optional) .....	15
4.2.5	Peristaltic pump connector (optional).....	15
4.2.6	Connecting the heat exchanger.....	16
4.2.7	Condensate drain connection .....	17
4.3	Electrical connections.....	17
4.4	Signal outputs .....	18
5	Operation and control .....	20
5.1	Description of functions.....	20
5.2	Delta T control option .....	20
5.3	Use of menu functions.....	21
5.3.1	Lock Menu.....	21
5.3.2	Overview of the menu items .....	22
5.4	Description of menu functions .....	24
5.4.1	Display menu.....	24
5.4.2	Main menu.....	24
5.4.3	Submenu 1.....	25
5.4.4	Submenu 1 (global settings).....	26
5.4.5	Set favourite menu.....	29
6	Maintenance.....	30
7	Service and repair.....	31
7.1	Troubleshooting .....	31
7.1.1	Error messages on the display.....	32
7.2	Safety instructions .....	33
7.3	Cleaning and removal of the heat exchanger.....	34
7.4	Replacing the hoses of the peristaltic pump (option) .....	34
7.5	Replacing the filter element (option) .....	34
7.6	Drying of the moisture detector (option).....	35
7.7	Calibration of the moisture detector (option) .....	35
7.8	Replacing sample gas pump inlet and outlet valves (optional) .....	35
7.9	Replacing the O-ring on the bypass valve (optional) .....	36
7.10	Replacing the bellow (optional) .....	36
7.11	Spare Parts.....	37
7.11.1	Consumables and accessories .....	37

7.11.2	Spare parts and accessories for cooler with -H2/-O2 heat exchanger .....	37
8	Disposal .....	38
9	Appendices .....	39
9.1	Gas cooler technical data .....	39
9.2	Technical Data - Options .....	42
9.3	Flow diagrams .....	43
9.4	Performance data.....	44
9.5	Heat exchanger .....	45
9.5.1	Heat exchanger description .....	45
9.5.2	Heat exchanger overview .....	46
9.6	Dimensions (mm) .....	48
10	Attached documents .....	51

# 1 Introduction

## 1.1 Intended use

This unit is intended for industrial use in gas analysis systems. It's an essential component for conditioning the sample gas to protect the analysis instrument from residual moisture in the sample gas.

Sample gas coolers with the option for high-purity oxygen (suffix -O2) are optimised especially for use with increased oxygen concentrations with regard to the parts in contact with the medium. Special cleaning of the components to minimise organic and inorganic contamination is mandatory. Manufacturing the products under controlled cleanliness conditions ensures compliance with the limit values in accordance with EIGA Doc 33/18.

Sample gas coolers with the option for high-purity hydrogen (suffix -H2) are specially refined using advanced manufacturing measures, in particular to prevent hydrogen-induced component damage. In addition, the parts in contact with the media are subjected to an additional visual inspection to remove any residual metallic contamination, such as chips and particles. Finally, a leak test is carried out as standard.

The device must not be operated in a zone 2, explosion class IIC (ATEX, IECEx and EAC Ex) explosive gas atmosphere which is rarely and only temporarily explosive, and in class I, division 2 (US & Canada).

For passing of flammable gases, make sure that the parts carrying and/or in contact with the medium are tightly connected.

Optional installation of various add-on equipment may limit the area of application of this device.

### Coolers with Canada certificate and IECEx

The device must be installed in a tool-secured IP54 housing.

### Coolers with USA certificate

The device must be installed in a tool-secured IP54 housing suitable for one or more class I division 2 wiring methods according to National Electric Code (ANSI/NFPA 70).

### Coolers with ATEX certificate

The device must be installed within a tool-secured enclosure providing a minimum degree of protection of IP54 and meeting the requirements of EN 60079-0 or certified as Ex e and in compliance with the enclosure, mounting, spacing and segregation requirements of the ultimate application.

### Coolers with EAC Ex certificate

The device must be installed in an IP54 rated housing which meets the requirements of GOST 14254-2015.

Please note the specifications in the data sheet on the specific intended use, existing material combinations, as well as pressure and temperature limits.

## 1.2 Overview

The TC-MIDI X2 series was designed specifically for high cooling capacities and high ambient temperatures.

The TC-MIDI+ X2 series was designed specifically for the requirements in so-called automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimise wash-out effects.

The TC-MIDI X2 with -H<sub>2</sub>/-O<sub>2</sub> heat exchanger series was specially developed for use with high-purity hydrogen and oxygen.

The Peltier coolers are distinguished by two types according to cooling capacity/operating temperature. This classification is reflected in the type designation. The exact item number of the model defined by you is determined by the model code in the ordering information category.

Application	Standard applications	
Operating temperature	40 °C	50 °C
1 heat exchanger (single or double)	TC-MIDI 6111 X2	TC-MIDI 6112 X2
1 heat exchanger for H <sub>2</sub> /O <sub>2</sub> applications	TC-MIDI 6111 X2	TC-MIDI 6112 X2
2 heat exchangers	TC-MIDI 6121 X2	TC-MIDI 6122 X2
2 heat exchangers in series	TC-MIDI+ 6121 X2	TC-MIDI+ 6122 X2


Additional components which every conditioning system should feature can optionally be integrated:

- Peristaltic pump for condensate separation,
- Filter,
- Moisture detector,
- Sample gas pump.

This allows for various configurations of cooler and options. Here the approach is to simplify creating a complete system in a cost-efficient way through pre-installed components with hoses connected. We further paid attention to easy access to wear parts and consumables.

## 1.3 Type plate

Example:

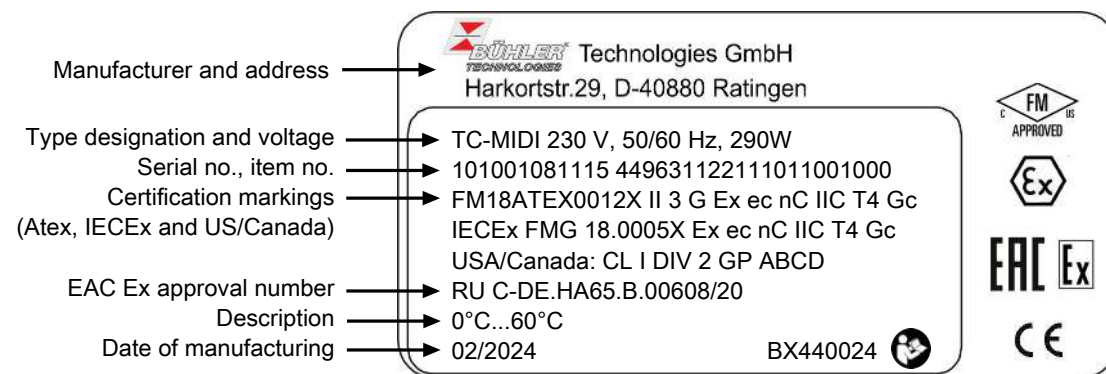

## 1.4 Scope of delivery

- Cooler
- Product documentation
- Connection-/mounting accessories (optional)

## 1.5 Ordering instructions

### 1.5.1 Gas cooler models with one gas path inside the heat exchanger

The item number is a code for the configuration of your unit. Please use the following model code:

4496	3	1	1	X	2	X	1	X	X	X	X	X	X	X	0	X	0	0	Product Characteristics
<b>Gas cooler models</b>																			
1																		TC-MIDI 6111 X2: Ambient temperature 40 °C	
2																		TC-MIDI 6112 X2: Ambient temperature 60 °C	
<b>Certifications</b>																			
2																		for explosive areas	
<b>Supply voltage</b>																			
1																		115 V AC, 50/60 Hz	
2																		230 V AC, 50/60 Hz	
<b>Heat exchanger</b>																			
1	1	0																Stainless steel, TS, metric	
1	1	5																Stainless steel, TS-I, US	
1	2	0																Duran glass, TG, metric	
1	2	5																Duran glass, TG-I, US	
1	3	0																PVDF, TV-SS, metric	
1	3	5																PVDF, TV-SS-I, US	
<b>Condensate drain <sup>2)</sup></b>																			
0																		without condensate drain	
1																		CPsingle X2 with hose nipple, angled	
3																		CPsingle X2 with screw connection <sup>4)</sup>	
<b>Sample gas pumps <sup>1)</sup></b>																			
0																		without sample gas pump	
1																		P1.3, PVDF, bottom mounted	
2																		P1.3, with bypass valve, bottom mounted	
6																		P1.3, PVDF, mounted externally	
7																		P1.3, with bypass valve, mounted externally	
<b>Moisture detector <sup>2)</sup> / Filter</b>																			
0	0																	without filter, without moisture detector	
0	1																	without filter, 1 moisture detector with PVDF adapter <sup>3)</sup>	
1	0																	1 filter, without moisture detector	
1	1																	1 filter with built-in moisture detector	
<b>Signal outputs</b>																			
0	0																	status output only	
1	0																	Analog output, 4...20 mA additional	
<b>Delta T control</b>																			
0	0																	without Delta T control	
1	0																	Delta T control option	

<sup>1)</sup> Factory installed tubing for suction operation.

<sup>2)</sup> With this option, the maximum ambient temperature is limited to 50 °C.

<sup>3)</sup> Also available in stainless steel.

<sup>4)</sup> Metric or US connection, per heat exchanger.

## 1.5.2 Gas cooler models with two gas paths inside the heat exchanger

The item number is a code for the configuration of your unit. Please use the following model code:

4496	3	1	1	X	2	X	2	X	X	X	X	X	X	0	X	0	0	Product Characteristics									
																		<b>Gas cooler models</b>									
1																		TC-MIDI 6111 X2: Ambient temperature 40 °C									
2																		TC-MIDI 6112 X2: Ambient temperature 60 °C									
																		<b>Certifications</b>									
2																		for explosive areas									
																		<b>Supply voltage</b>									
1																		115 V AC, 50/60 Hz									
2																		230 V AC, 50/60 Hz									
																		<b>Heat exchanger</b>									
				2	6	0												Stainless steel, DTS, metric									
				2	6	5												Stainless steel, DTS-I, US									
				2	6	1												Stainless steel, DTS 6, metric <sup>1)</sup>									
				2	6	6												Stainless steel, DTS 6-I, US <sup>1)</sup>									
				2	7	0												Duran glass, DTG, metric									
				2	7	5												Duran glass, DTG-I, US									
				2	8	0												PVDF, DTV, metric <sup>1)</sup>									
				2	8	5												PVDF, DTV-I, US <sup>1)</sup>									
																		<b>Condensate drain</b> <sup>4)</sup>									
				0														without condensate drain									
				2														CPdouble X2 with hose nipple, angled									
				4														CPdouble X2 with screw connection <sup>6)</sup>									
																		<b>Sample gas pumps</b> <sup>3)</sup>									
				0														without sample gas pump									
				1														P1.3, 1 gas path, PVDF, bottom mounted									
				2														P1.3, 1 gas path, with bypass valve, bottom mounted									
				6														P1.3, 1 gas path, PVDF, mounted externally <sup>2)</sup>									
				7														P1.3, 1 gas path, with bypass valve, mounted externally <sup>2)</sup>									
																		<b>Moisture detector</b> <sup>4)</sup> / <b>Filter</b>									
				0	0													without filter, without moisture detector									
				0	1													without filter, 1 moisture detector with PVDF adapter <sup>5)</sup>									
				0	2													without filter, 2 moisture detectors with PVDF adapter <sup>5)</sup>									
				1	0													1 filter, without moisture detector									
				1	1													1 filter with built-in moisture detector									
				2	0													2 filters, without moisture detector <sup>2)</sup>									
				2	1													2 filters, 1 moisture detector <sup>2)</sup>									
				2	2													2 filters, 2 moisture detectors <sup>2)</sup>									
																		<b>Signal outputs</b>									
				0	0													status output only									
				1	0													Analog output, 4...20 mA additional									
																		<b>Delta T control</b>									
				0	0													without Delta T control									
				1	0													Delta T control option									

<sup>1)</sup> Condensate outlets only suitable when connecting peristaltic pumps.

<sup>2)</sup> External sample gas pump P1.3 only allows 1 filter.

<sup>3)</sup> Factory installed tubing for suction operation.

<sup>4)</sup> With this option, the maximum ambient temperature is limited to 50 °C.

<sup>5)</sup> Also available in stainless steel.

<sup>6)</sup> Metric or US connection, per heat exchanger.



### 1.5.3 Gas cooler models with one or two gas paths in the heat exchanger for H2/O2 applications

The item number is a code for the configuration of your unit. Please use the following model code:

4496	3	1	1	X	2	X	X	X	X	0	0	0	0	X	0	X	0	X	Product Characteristics
<b>Gas cooler models</b>																			
1																		TC-MIDI 6111 X2: Ambient temperature 40 °C	
2																		TC-MIDI 6112 X2: Ambient temperature 60 °C	
<b>Certifications</b>																			
2																		for explosive areas	
<b>Supply voltage</b>																			
1																		115 V AC, 50/60 Hz	
2																		230 V AC, 50/60 Hz	
<b>Heat exchanger</b>																			
1	1	0																-O2 Stainless steel, TS-O2, metric	
1	1	5																-O2 Stainless steel, TS-I-O2, US	
1	1	0																-H2 Stainless steel, TS-H2, metric	
1	1	5																-H2 Stainless steel, TS-I-H2, US	
2	6	0																-O2 Stainless steel, DTS-O2, metric	
2	6	5																-O2 Stainless steel, DTS-I-O2, US	
2	6	0																-H2 Stainless steel, DTS-H2, metric	
2	6	5																-H2 Stainless steel, DTS-I-H2, US	
<b>Signal outputs</b>																			
										0	0							status output only	
										1	0							Analog output, 4..20 mA, incl. status output	
<b>Delta T control</b>																			
										0	0							without Delta T control	
										1	0							Delta T control option	

## 1.5.4 Gas cooler models with two heat exchangers

The item number is a code for the configuration of your unit. Please use the following model code:

4496	3	1	2	X	2	X	2	X	X	X	X	X	X	0	X	0	0	Product Characteristics												
																			<b>Gas cooler models</b>											
																			TC-MIDI 6121 X2: Ambient temperature 40 °C											
																			TC-MIDI 6122 X2: Ambient temperature 60 °C											
																			<b>Certifications</b>											
																			for explosive areas											
																			<b>Supply voltage</b>											
																			115 V AC, 50/60 Hz											
																			230 V AC, 50/60 Hz											
																			<b>Heat exchanger</b>											
																			Duran glass, STG-2, metric											
																			Duran glass, STG-2-I, US											
																			PVDF, STV-2, metric <sup>1)</sup>											
																			PVDF, STV-2-I, US <sup>1)</sup>											
																			<b>Condensate drain</b> <sup>4)</sup>											
																			without condensate drain											
																			CPdouble X2 with hose nipple, angled											
																			CPdouble X2 with screw connection <sup>6)</sup>											
																			<b>Sample gas pumps</b> <sup>3)</sup>											
																			without sample gas pump											
																			P1.3, 1 gas path, PVDF, bottom mounted											
																			P1.3, 1 gas path, with bypass valve, bottom mounted											
																			P1.3, 1 gas path, PVDF, mounted externally <sup>2)</sup>											
																			P1.3, 1 gas path, with bypass valve, mounted externally <sup>2)</sup>											
																			<b>Moisture detector</b> <sup>4)</sup> / <b>Filter</b>											
																			without filter, without moisture detector											
																			without filter, 1 moisture detector with PVDF adapter <sup>5)</sup>											
																			1 filter, without moisture detector											
																			1 filter with built-in moisture detector											
																			<b>Signal outputs</b>											
																			status output only											
																			Analog output, 4...20 mA additional											
																			<b>Delta T control</b>											
																			without Delta T control											
																			Delta T control option											

<sup>1)</sup> Condensate outlets only suitable when connecting peristaltic pumps.

<sup>2)</sup> External sample gas pump P1.3 only allows 1 filter.

<sup>3)</sup> Factory installed tubing for suction operation.

<sup>4)</sup> With this option, the maximum ambient temperature is limited to 50 °C.

<sup>5)</sup> Also available in stainless steel.

<sup>6)</sup> Metric or US connection, per heat exchanger.

## 1.5.5 Gas cooler models with two heat exchangers in series

The item number is a code for the configuration of your unit. Please use the following model code:

4496	3	1	2	X	2	X	1	X	X	X	X	X	X	0	0	0	0	Product Characteristics	
																		<b>Gas cooler models</b>	
1																		TC-MIDI+ 6121 X2: Ambient temperature 40 °C	
2																		TC-MIDI+ 6122 X2: Ambient temperature 60 °C	
																		<b>Certifications</b>	
2																		for explosive areas	
																		<b>Supply voltage</b>	
1																		115 V AC, 50/60 Hz	
2																		230 V AC, 50/60 Hz	
																		<b>Heat exchanger</b>	
		1	2	2														Duran glass, STG-2, metric	
		1	2	7														Duran glass, STG-2-I, US	
		1	3	2														PVDF, STV-2, metric <sup>1)</sup>	
		1	3	7														PVDF, STV-2-I, US <sup>1)</sup>	
																		<b>Condensate drain</b> <sup>4)</sup>	
		0																without condensate drain	
		2																CPdouble X2 with hose nipple, angled	
		4																CPdouble X2 with screw connection <sup>6)</sup>	
																		<b>Sample gas pumps</b> <sup>3)</sup>	
		0																without sample gas pump	
		1																P1.3, 1 gas path, PVDF, bottom mounted	
		2																P1.3, 1 gas path, with bypass valve, bottom mounted	
		6																P1.3, 1 gas path, PVDF, mounted externally <sup>2)</sup>	
		7																P1.3, 1 gas path, with bypass valve, mounted externally <sup>2)</sup>	
																		<b>Moisture detector</b> <sup>4)</sup> / <b>Filter</b>	
		0	0															without filter, without moisture detector	
		0	1															without filter, 1 moisture detector with PVDF adapter <sup>5)</sup>	
		1	0															1 filter, without moisture detector	
		1	1															1 filter with built-in moisture detector	
																		<b>Signal outputs</b>	
		0	0															status output only	
		1	0															Analog output, 4...20 mA additional	

<sup>1)</sup> Condensate outlets only suitable when connecting peristaltic pumps.

<sup>2)</sup> External sample gas pump P1.3 only allows 1 filter.

<sup>3)</sup> Factory installed tubing for suction operation.

<sup>4)</sup> With this option, the maximum ambient temperature is limited to 50 °C.

<sup>5)</sup> Also available in stainless steel.

<sup>6)</sup> Metric or US connection, per heat exchanger.

## 2 Safety instructions

### 2.1 Important notices

**NOTICE**

**The device is suitable for hazardous areas.**

This unit may only be used if:

- The product is being used under the conditions described in the operating- and installation instructions, used according to the nameplate and for applications for which it is intended. Any unauthorized modifications to the unit will void the warranty provided by Bühler Technologies GmbH,
- The specifications and markings in the type plate must be observed,
- The threshold values in the data sheet and the instructions must be observed,
- Monitoring equipment / protection devices must be connected correctly,
- Service and repair work not described in these instructions are performed by Bühler Technologies GmbH,
- Genuine replacement parts must be used.

Erecting electrical systems in explosive areas requires compliance with the following national regulations:

- IEC/EN 60079-14
- National electric code (NEC)
- Canadian electric code (CEC)

Additional national regulations pertaining to initial operation, operation, maintenance, repairs and disposal must be observed.

These operating instructions are a part of the equipment. The manufacturer reserves the right to change performance-, specification- or technical data without prior notice. Please keep these instructions for future reference.

### Signal words for warnings

**DANGER**

Signal word for an imminent danger with high risk, resulting in severe injuries or death if not avoided.

**WARNING**

Signal word for a hazardous situation with medium risk, possibly resulting in severe injuries or death if not avoided.

**CAUTION**

Signal word for a hazardous situation with low risk, resulting in damaged to the device or the property or minor or medium injuries if not avoided.

**NOTICE**

Signal word for important information to the product.

## Warning signs

These instructions include the following warnings:



General warning sign



General mandatory sign



Voltage warning



Unplug from mains



Warning not to inhale toxic gases



Wear respiratory equipment



Warning of corrosive substances



Wear a safety mask



Warning of explosion hazard



Wear gloves



Warning of hot surfaces

## 2.2 General hazard warnings

The equipment must be installed by a professional familiar with the safety requirements and risks.

Be sure to observe the safety regulations and generally applicable rules of technology relevant for the installation site. Prevent malfunctions and avoid personal injuries and property damage.

### The operator of the system must ensure:

- Safety notices and operating instructions are available and observed,
- The respective national accident prevention regulations are observed,
- The permissible data and operational conditions are maintained,
- Safety guards are used and mandatory maintenance is performed,
- Legal regulations are observed during disposal,
- compliance with national installation regulations.

### Maintenance, Repair

Please note during maintenance and repairs:

- Repairs to the unit must be performed by Bühler authorised personnel.
- Only perform conversion-, maintenance or installation work described in these operating and installation instructions.
- Always use genuine spare parts.
- Do not install damaged or defective spare part. If necessary, visually inspect prior to installation to determine any obvious damage to the spare parts.

Always observe the applicable safety and operating regulations in the respective country of use when performing any type of maintenance.

#### DANGER

#### Electrical voltage

Electrocution hazard.

- a) Disconnect the device from power supply.
- b) Make sure that the equipment cannot be reconnected to mains unintentionally.
- c) The device must be opened by trained staff only.
- d) Regard correct mains voltage.



**DANGER**

**Toxic, corrosive gas/condensate**



Sample gas/condensate may be hazardous to health.

- a) If necessary, ensure a safe gas/condensate discharge.
- b) Always disconnect the gas supply when performing maintenance or repairs.
- c) Protect yourself from toxic/corrosive gasses/condensate when performing maintenance. Wear appropriate protective equipment.



**DANGER**

**Explosion hazard**



Life and explosion risk may result from gas leakage due to improper use.

- a) Use the devices only as described in this manual.
- b) Regard the process conditions.
- c) Check tubes and hoses for leakage.

**WARNING**

**Risk of breakage**



- a) Protect the equipment against being hit.
- b) Protect the device against falling objects.

## 3 Transport and storage

Only transport the product inside the original packaging or a suitable alternative.

The equipment must be protected from moisture and heat when not in use. It must be stored in a covered, dry and dust-free room at a temperature of -20 °C to 60 °C (-4 °F to 140 °F).

In particular for sample gas coolers with stainless steel heat exchangers for  $O_2$  applications (suffix -O2), it is essential to rule out any contamination of components in contact with the media during storage.

## 4 Installation and connection

### 4.1 Installation site requirements

The unit is only intended for wall-mounted use in enclosed areas. Adequate protection from the weather must be provided when used outdoors.

Install the unit leaving enough room below the cooler to discharge the condensate. Leave room above for the gas supply.

Be sure to maintain the approved ambient temperature. Do not obstruct the convection of the cooler. The vents must have enough room to the next obstacle. The distance must especially be a minimum of 10 cm on the air outlet side.

Ensure adequate ventilation when installing in enclosed housings, e.g. analyser cabinets. If the convection is inadequate, we recommend aerating the cabinet or installing a fan to lower the inside temperature.

#### CAUTION



#### Contamination of cleaned components

For sample gas coolers with stainless steel heat exchangers for O<sub>2</sub> applications (suffix -O<sub>2</sub>), contamination with oil, grease, dust, particles, lint, hair, etc. must be ruled out for fire protection reasons when working on components that come into contact with media. If necessary, adapt your operational and organisational measures with regard to the work clothing to be used, hygiene regulations, etc. If necessary, move such work to a suitable, cleaner work area.



### 4.2 Installation

Run the gas supply to the cooler with a downward slope. The gas inputs are marked in red and additionally labelled "IN".

If a large amount of condensate accumulates, we recommend using a condensate trap with automatic condensate drain. Our condensate drains, 11 LD V38, AK 20, AK 5.5 OR AK 5.2, are suitable.

Glass vessels and automatic condensate drains are available for draining condensate for external mounting below the unit. When using automatic condensate drains, the sample gas pump must be installed upstream of the cooler (pressure operation) to ensure proper function of the condensate drain.

If the sample gas pump is located at the cooler outlet (suction operation), we recommend using glass condensate traps or peristaltic pumps.

With the option for high-purity water or oxygen (suffix -H<sub>2</sub>/-O<sub>2</sub>), the components are each supplied in separate packaging. To prevent soiling, these should only be unpacked shortly before use.

#### Installation instructions additional type plate -H<sub>2</sub>:

To ensure traceability of the leakage test of the heat exchanger in H<sub>2</sub> applications, affix the enclosed additional type plate in a suitable place before commissioning. When affixing to the cooler housing, no openings must be closed, and overlapping with other stickers or components is not permitted – minimum distance: 20 mm.

#### CAUTION



#### Warning of electrical charge (-H<sub>2</sub>)

When affixing to the cooler:  
The enclosed additional type plate of the heat exchanger must be affixed to the cooler according to the installation instructions.



### 4.2.1 Connecting the filter gas connections (optional)

The connection between the heat exchanger outlet and the filter inlet does not have tubing included. The connection G1/4 or NPT 1/4" (filter head marked NPT) for the gas outlet must be carefully and properly connected using a suitable screw connection.

When ordering the cooler with the **option filter without Moisture detector**, a bypass may be connected to the filter head.

The filter head is intended for a G1/4 internal screw thread which is plugged at the factory. To use it, unscrew the plug and screw in a suitable screw connection. Pay attention to leaks.

#### NOTICE



Installing **filters** limits the maximum approved **operating pressure** in the system!  
Operating pressure ≤ 2 bar

### 4.2.2 Flow adapter connection (optional)

When ordering the cooler with the **option moisture detector without filter**, it will be factory installed inside a flow adapter.

The connection between the heat exchanger outlet and the flow adapter inlet already has tubing. The connection G 1/4 or NPT 1/4" (flow adapter marked NPT) for the gas outlet must be carefully and properly connected using a suitable screw connection.

### 4.2.3 Connecting the moisture detector (option)

When ordering the cooler with **moisture detector option**, it will be factory installed inside a flow adapter, or for the **filter option** installed and connected in the filter head.

### 4.2.4 Sample gas pump connection gas lines (optional)

On coolers ordered with attached sample gas pump these are already installed and wired. Add-on parts ordered at the same time are already installed and connected to the sample gas pump.

The sample gas pump may be installed both below and next to the cooler.

Avoid mixed-material installation, i.e. metal piping to plastic bodies. If this cannot be avoided in isolated applications, screw the metal connections into the pump body with care, never use force.

Lay the lines so the line at the inlet and outlet remains flexible for an adequate distance.

The pumps are marked **IN** for inlet and **OUT** for outlet at the mounting ring. Be sure the gas line connections are tight.

### 4.2.5 Peristaltic pump connector (optional)

Coolers ordered with attached peristaltic pump already have it installed and wired. Heat exchangers ordered at the same time are already installed and connected to the peristaltic pump.

The ø6 mm (0.24 inch) hose nipple for the pump's condensate outlet must be carefully and properly connected with a suitable hose and hose clamp.

Versions with screw connections DN 4/6 or 1/6"-1/4" are supplied with ferrule and knurled nut and must be carefully sealed with appropriate hose.

#### NOTICE




Installing peristaltic **pumps** CPsingle / CPdouble limits the maximum permissible **operating pressure** in the system!  
Operating pressure ≤ 1 bar

## 4.2.6 Connecting the heat exchanger

The picture on the left shows the schematics for connecting (two) separate heat exchangers.


To minimise gas wash out in the cooler, the two (identical) heat exchangers must be operated in series (right picture). This should be done as follows:

1. Gas inlet line to red gas inlet on heat exchanger 2 (pre-cooling).
2. Connection between gas outlet on heat exchanger 2 and the red gas inlet on heat exchanger 1 (after-cooling).
3. Attaching the final gas output line to the gas outlet on heat exchanger 1.

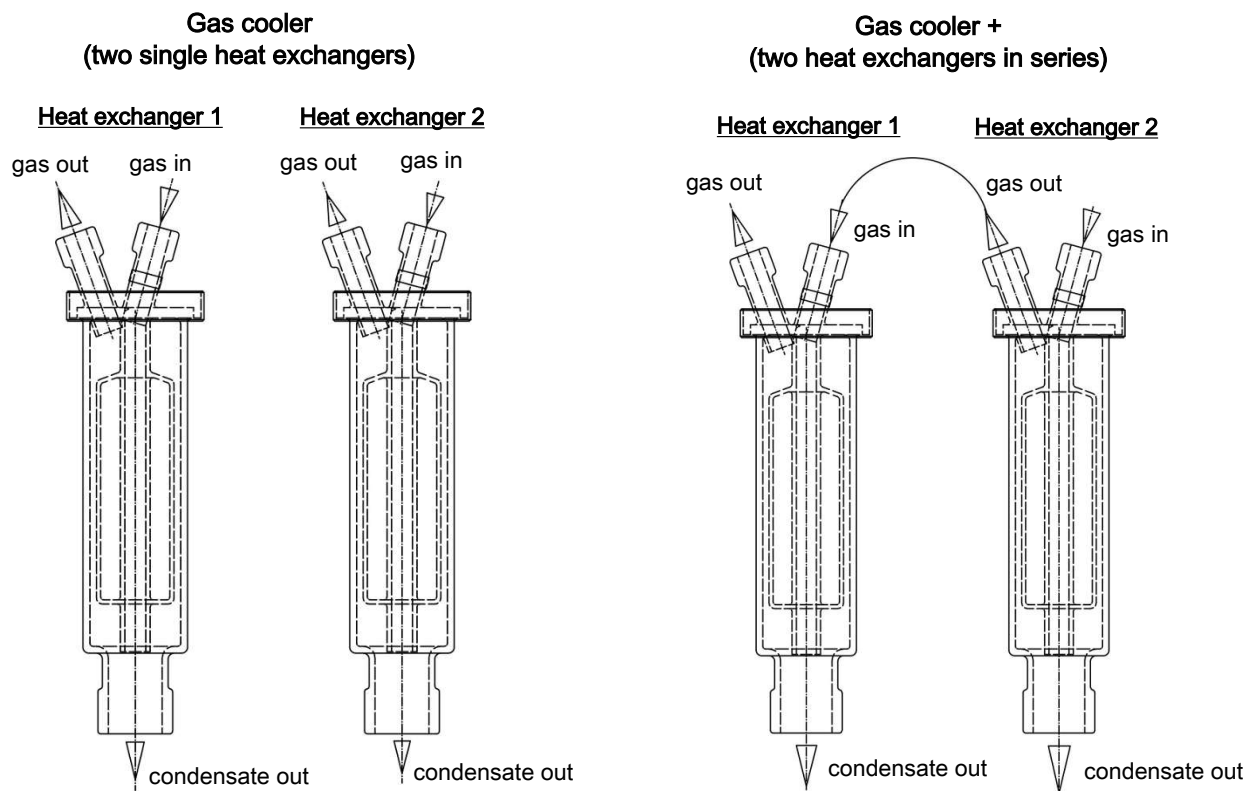

The gas inputs are marked in red.

On glass heat exchangers, the correct position of the seal is important when connecting the gas lines (see image). The seal consists of a silicone ring with a PTFE sleeve. The PTFE side must face the glass thread.

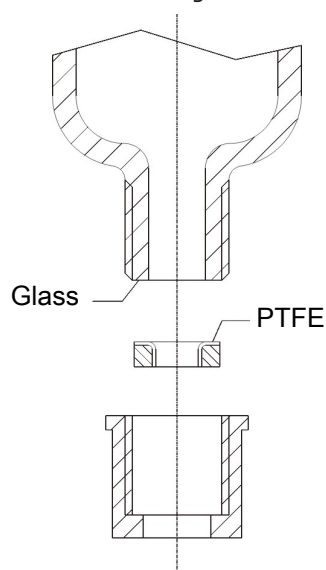

Pay attention to the appropriate spanner size when selecting fittings for stainless steel heat exchangers.

TS/TS-I gas connections: SW 17

TS/TS-I condensate out connections: SW 22

## 4.2.7 Condensate drain connection

Depending on the material, build a connecting line with fittings and tubing or hose between the heat exchanger and condensate drain. For stainless steel, the condensate drain can be hung directly from the connecting tube; for hoses, the condensate drain must be secured separately using a clamp.

The condensate drain can be mounted directly to the heat exchanger.

When choosing the option for high-purity oxygen, make sure to select the suffix -O2.

If the condensate drain 11 LD V 38 is used for high hydrogen concentrations, the system in which it is installed must be tested for leaks.

Condensate lines must always be installed with a slope and a minimum inside diameter of DN 8/10 (5/16").

## 4.3 Electrical connections

The operator must install an external separator for the device which is clearly assigned to this device.

This separator

- must be located near the device,
- must be easy for the operator to reach,
- must comply with IEC 60947-1 and IEC 60947-3,
- must separate all live conductors and the status output, and
- must not be attached to the power feed.

The mains supply of the device must be fused according to the specifications under technical data.

### Potential equalization/static charge

Static charges can result in incendive sparking. Avoid static charges. Any conductive parts of the cooler must be grounded!

The housing has a connection for an earth/equipotential bonding conductor. Ensure the housing is adequately earthed (minimum conductor cross-section 4 mm<sup>2</sup>).

Particularly observe the requirements of EN 60079-14!

#### WARNING



#### Hazardous electrical voltage

The device must be installed by trained staff only.

#### CAUTION



#### Wrong mains voltage

Wrong mains voltage may damage the device.  
Regard the correct mains voltage as given on the type plate.

#### WARNING



#### High voltage

Damage to the device in case of insulation testing  
**Do not proceed insulation tests with high voltage** to the device as a whole!

### Electric strength test


This device is equipped with extensive EMC protection. The necessary tests were carried out at the factory (test voltage 2.1 kV or 2.55 kV DC depending on approval).

If you wish to check the electric strength again yourself, you can do so on the entire unit. Only test the device with the specified values using direct current voltage. Testing the electric strength with alternating current voltage will damage electronic components. The recommended voltage in this case is 2.1 kV DC, 2 s. Disconnect all supply lines from the device before testing. Power can be supplied via the mains connection.

## Plug connection

This device has one EN 175301-803 plug each for the power supply and the signal output. If the lead is connected correctly, these cannot be confused. Therefore please be sure to correctly reassemble the plugs after connecting the wires. Below you will find the pin assignments, with the numbers corresponding to those on the plugs:

The supply line cross-sections must be suitable for the rated current. Use a maximum line cross-section of 1.5 mm<sup>2</sup> (AWG 16) and a cable diameter of 8 - 10 mm (0.31 - 0.39 inch).

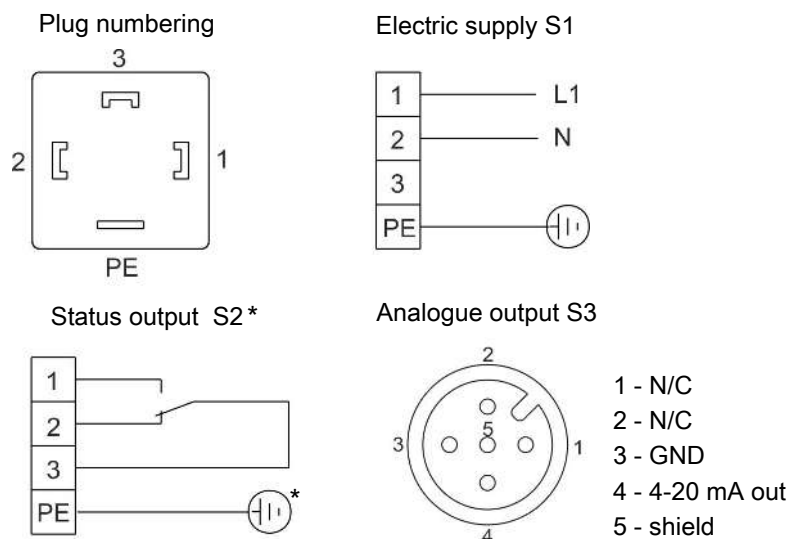

\* When using the status output with voltage  $\geq 33$  V AC or  $\geq 70$  V DC, the protective earth conductor (PE) must be connected.

The clamping areas for S1 and S2 are 8–10 mm (0.31–0.39 inches) in diameter.

## 4.4 Signal outputs

The device provides different status signals. The maximum switching load of the status outputs is limited to 250 V AC/150 V DC, 2 A, 50 VA each.

An alarm is triggered by the status output (S2) if the temperature of the cooler is outside the specified limits. It does not indicate if the alarm was triggered due to excess temperature or insufficient temperature.

The front film has three LEDs:

Colour	Marking	Function
Red	S2	High/low temperature, device error
Yellow	S1	---
Green	OP	Normal operation

The LEDs OP and S2 indicate the device status similar to the status output S2.

If the option “temperature signal” is built in, the unit has a signal output via the analogue output to indicate the actual cooler temperature.

When the moisture detector (optional) is installed, an alarm is activated by the status output (S2) if the moisture is still present in the prepared sample gas. Thereby, no distinction is made between the alarm/cable break triggered by moisture detector 1 or 2. This information is displayed by an error message instead.

The temperature signal can be read via the panel plug (S3) using the M12x1 connector. This plug is located next to the moisture detector connectors at the top of the cooler.

## Description of signal outputs

	Function/contact type	Description	
Regarding S2)	internal changeover contact: max. 250 V AC/ 150 V DC, 2 A, 50 VA	the following device statuses can be indicated via two switching outputs:	<p>Contact between 3 and 2 closed (alarm)</p> <ul style="list-style-type: none"> <li>– No mains voltage and/or actual temperature outside the alarm thresholds</li> </ul> <p>Contact between 3 and 1 closed (ok)</p> <ul style="list-style-type: none"> <li>– Mains voltage attached + actual temperature within the alarm thresholds</li> </ul> <p><b>with moisture detector option</b></p> <p>Contact between 3 and 2 closed (alarm)</p> <ul style="list-style-type: none"> <li>– The moisture detector registers residual humidity in the sample gas or cable break: Error message</li> </ul> <p>Contact between 1 and 3 closed (ok)</p> <ul style="list-style-type: none"> <li>– no residual moisture in measuring gas/no cable break</li> </ul>
Regarding S3)	4-20 mA analogue output ( $R_{load} < 500 \Omega$ )	Signalling of actual temperature (please use shielded cables)	<p><math>T_{Cooler} = -20 \text{ °C } \triangle (-4 \text{ °F}) \rightarrow 4 \text{ mA} / 2 \text{ V}</math></p> <p><math>T_{Cooler} = 5 \text{ °C } \triangle (41 \text{ °F}) \rightarrow 9 \text{ mA} / 4,5 \text{ V}</math></p> <p><math>T_{Cooler} = 60 \text{ °C } \triangle (140 \text{ °F}) \rightarrow 20 \text{ mA} / 10 \text{ V}</math></p>

## 5 Operation and control

### NOTICE



The device must not be operated beyond its specifications.

After switching on the cooler the block temperature will be displayed. The display will flash until the block temperature has reached the preset target value ( $\pm$  adjustable alarm range). The status contact is in the Alarm position.

Once the target temperature range has been reached, the temperature will continuously be displayed and the status contact switches over.

If the display flashes during operation or an error message appears, please refer to bullet "Troubleshooting".

Please refer to the data sheet for performance data and maximum ratings.

### 5.1 Description of functions

The cooler is controlled by a microprocessor. With the factory preset the control already incorporates the various characteristics of the built-in heat exchangers.

The programmable display shows the block temperature in the selected display unit ( $^{\circ}\text{C}$  /  $^{\circ}\text{F}$ ) (factory preset  $^{\circ}\text{C}$ ). Application-specific settings can easily be configured guided by the menu, using the 5 buttons. For one, this applies to the target outlet dew point, which can be set from 2 to 20  $^{\circ}\text{C}$  (36  $^{\circ}\text{F}$  to 68  $^{\circ}\text{F}$ ) (factory preset 5  $^{\circ}\text{C}$ /41  $^{\circ}\text{F}$ ).

And then the warning thresholds can be adjusted for low and excess temperature. These are set relative to the outlet dew point  $\tau_a$  setting.

For the low temperature the range is  $\tau_a - 1$  to  $- 3$  K (at a minimum 1  $^{\circ}\text{C}$ / 34  $^{\circ}\text{F}$  cooling block temperature), for the excess temperature the range is  $\tau_a + 1$  to  $+ 7$  K. The factory presets for both values are 3 K.

The flashing display and the status relays indicate the conditions are below or above the configured warning range (e.g. after switching on).

The status output can e.g. be used to control the sample gas pump to allow for the gas flow to only be switched on once the permissible cooling range has been reached or shut off the pump in the event of a moisture detector alarm.

The separated condensate can be drained via connected peristaltic pumps or add-on automatic condensate drains.

Fine mesh filters can also be used, which in turn can be installed in optional moisture detectors.

The glass dome allows the dirt level of the filter element to easily be determined.

The moisture detector is easy to remove. This may be required if a condensate enters the cooler due to a malfunction and the peristaltic pump or the automatic condensate drain is unable to remove it.

A P1 gas pump can be attached to the gas cooler, optionally also with bypass valve for regulating the flow. This allows the sample gas pump to be expanded by a single-leg system, so when equipped with a single heat exchanger or for the respective application the two gas paths of the dual heat exchangers are switched in series, for example Cooling 1 – Pump – Cooling 2.

### 5.2 Delta T control option

Not all applications require an outlet dew point of 5  $^{\circ}\text{C}$  (41  $^{\circ}\text{F}$ ). In some applications a higher dew point is sufficient. In other applications a stable outlet dew point doesn't matter, it's enough for the gas to be dry, so if the outlet dew point has an adequate difference in temperature below the ambient temperature.

Here the electronics measure the ambient temperature and regulate the outlet dew point to an adjustable value below it. This extends the potential cooling capacity to the limits of the heat exchanger. Here it's important to note the outlet dew point fluctuates along with the ambient temperature and a stable dew point cannot be a prerequisite for the measurement.

The target temperature range is defined by the ambient temperature, the adjustable temperature difference and the alarm limits. If the block temperature is not within the target range with active Delta T-control, the status message "**dt**" will flash in the display.

**Example:** At a difference of 30  $^{\circ}\text{C}$  (30 K/54  $^{\circ}\text{F}$ ), at a set outlet dew point of 5  $^{\circ}\text{C}$  (41  $^{\circ}\text{F}$ ) this means the dew point remains stable up to an ambient temperature of approx. 35  $^{\circ}\text{C}$  (95  $^{\circ}\text{F}$ ), and the safe drop is only preferred over the ambient temperature with ambient temperature peaks over 35  $^{\circ}\text{C}$  (95  $^{\circ}\text{F}$ ). The cooling capacity specified in the cooling capacity graphs at 35  $^{\circ}\text{C}$  (95  $^{\circ}\text{F}$ ) is then available at above 35  $^{\circ}\text{C}$  (95  $^{\circ}\text{F}$ ).

## 5.3 Use of menu functions

### Brief description of the operating principle:

The unit is operated using 5 keys. Their functions are:

Button	Section	Functions
← or OK	Display	– Switches from the measurement display to the main menu
	Menu	– Selects the menu item displayed
	Enter	– Applies an edited value or a selection
▲	Display	– temporarily switches to the alternative measurement display (if option installed)
	Menu	– Back
	Enter	– Increase value or browse selection – Note: – Press button 1 x = changes parameter / value by one; – Hold button = fast mode (numerical values only) – Display flashes: modified parameter/value – Steady display: original display/value
▼	Display	– temporarily switches to the alternative measurement display (if option installed)
	Menu	– Next
	Enter	– Reduce value or browse selection
ESC	Menu	– Move one level up
	Enter	– Return to menu Changes will not be saved!
F or Func		– Sets a menu to favourite. (Note: The favourite menu will also be activated with the menu locked!)

### 5.3.1 Lock Menu

Some menus can be locked to prevent inadvertently changing the settings of the unit. This requires setting a code. For information on setting up or disabling the menu lock please refer to "Global Settings" (*tOP*) under menu item *tOP* > *Loc*.

The menu lock is **not** enabled at the time of delivery, all menu items can be accessed.

With the menu locked, only the following menu items will be visible without entering the correct code:

Menu item	Explanation
<i>tOP</i> > <i>uni</i> <i>t</i>	Temperature unit selection (°C or °F).
F or Func.	Accessing the Favourites menu
	<b>NOTICE! This menu may be one that is normally locked.</b>

### 5.3.2 Overview of the menu items

When pressing the **OK** button in normal mode, the display will show the prompt **codE** if the menu is locked. Use the **▲** and **▼** buttons to enter the correct code and press **OK**.

If an incorrect code or no code is entered, the menu will not be unlocked and you will not be able to access all menu items.

If you forgot the password you can always enter master code 287 to access the menu; the menu will be unlocked.


The following image shows an overview of the menu structure.

Items with a dashed frame will only appear with the respective settings or with the respective status messages.

The factory defaults and settings ranges are specified in the overview as well as under the respective menu item. The factory defaults apply unless otherwise agreed.


You can cancel entries and menu selections without saving by pressing the **ESC** key.

#### Menu:




1. Menu designation
2. Display
3. Brief description

#### Parameter:



4. Value input
5. Factory preset
6. Parameter range



7. Selecting from the list of values
8. Factory preset
9. Parameter range/selection

#### Optional menu navigation:



10. dashed box = Optional



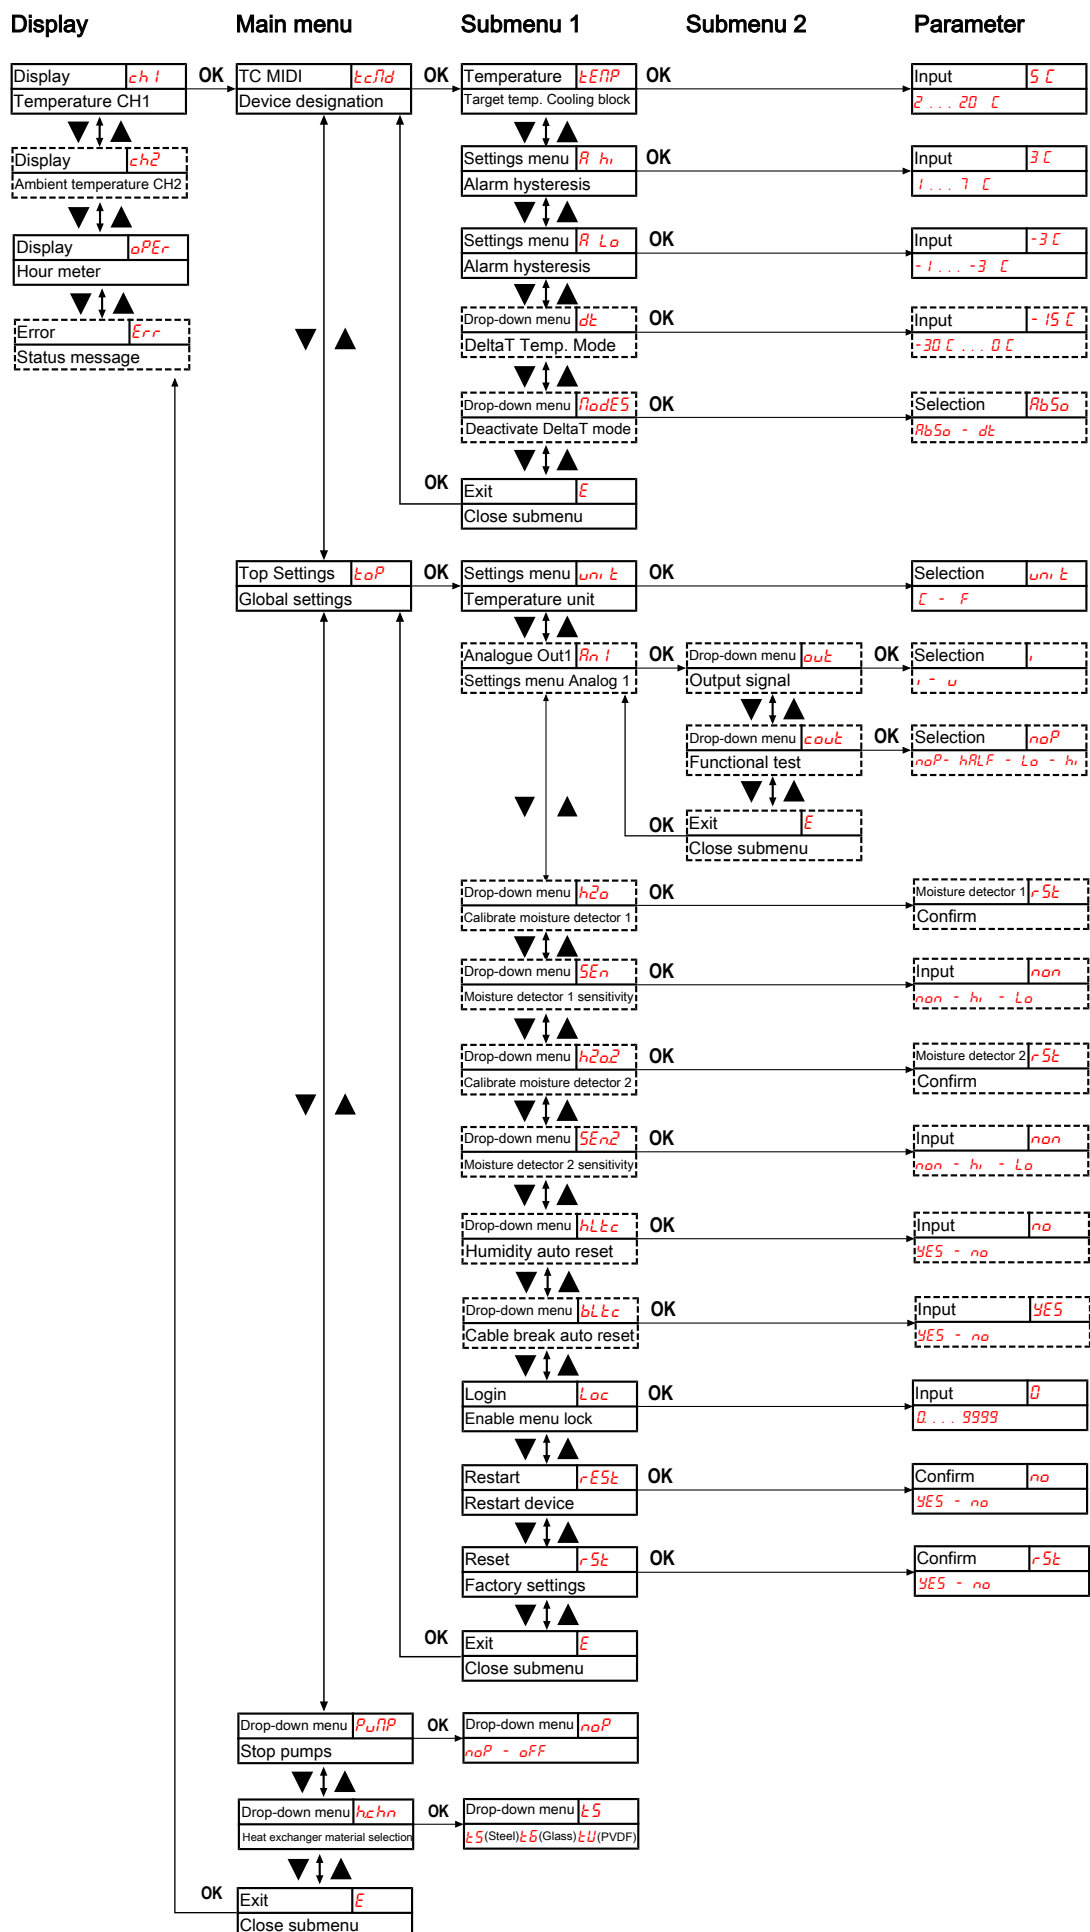



Fig. 1: Menu overview TC MIDI

## 5.4 Description of menu functions

### 5.4.1 Display menu

#### Block temperature display

Display → *ch1*



Depending on the device state, the temperature will be displayed as a constant, flashing, or alternating with a status message.

#### Ambient temperature display

Display → *ch2*



The display is only available on devices with „Delta-T“ option. Depending on the device state, the temperature will be displayed as a constant, flashing, or alternating with a status message.

#### Operating hours /runtime display

Display → *oPEr*




Displays the operating hours of the unit. The runtime cannot be reset and can be output in various display formats. To view/exit the runtime, press the „Enter“ key.

- *yyMM* – display in years and months (default)
- *MMh* – display in months
- *WEEh* – display in weeks
- *dDYS* – display in days
- One month corresponds to 30 days. Press the „F“ key to switch between the display formats. The display will then first show the selected format as short text, then the duration.

#### Error code display

Display → *Err*



In the event of errors/malfunctions not related to operation, the error code indicates possible causes and solutions.

### 5.4.2 Main menu

#### Peltier Cooler TC-MIDI

Display → *tcMId*



This will take you to the cooler target temperature and the tolerance range setting (alarm threshold).

#### Global setting


Display → *LoP* (ToP Settings)



This menu is used to configure the global cooler settings.

## Peristaltic pump and sample gas pump

Display → **PuRP**



Switching the peristaltic pump and sample gas pump on and off.

Parameter range: **noP**, **oFF**

Factory setting: **noP**

Note: Status switches, "PuRP" flashes.

## Heat exchanger material selection

Display → **hchh**



Heat exchanger material selection

Parameter range: **LS** (Steel), **LG** (Glass), **LU** (PVDF)

Factory setting: **LS** (cooler without heat exchanger), or respective material per configuration

## Exit main menu

Display → **E**



Selecting this will return you to display mode.

## 5.4.3 Submenu 1

### Target temperature

Display → Cooler → **LEMP**



This setting determines the nominal temperature for the cooler temperature.

Parameter range: 2 °C to 20 °C (35.6 °F to 68 °F)


Factory setting: 5 °C (41 °F)

Note: If the temperature is changed the indicator may blink, until the new operating range has been reached.

This menu item is hidden if the keylock is enabled.

### upper alarm limit

Display → Cooler → **A hi** (Alarm high)



Here you can set the upper threshold for the visual signal and the status relay. The alarm limit is set based on the cooler temperature setting.

Parameter range: 1 °C to 7 °C (1.8 °F to 12.6 °F)

Factory setting: 3 °C (5.4 °F)

Note: This menu item is hidden if the keylock is enabled.


**lower alarm limit**Display → Cooler → *R Lo* (Alarm low)

Here you can set the lower threshold for the visual signal and the status relay. The alarm limit is set based on the cooler temperature setting.

Parameter range: -1 °C to -3 °C (-1.8 °F to -5.4 °F)

Factory setting: -3 °C (-5.4 °F)

Note: This menu item is hidden if the keylock is enabled.


**DeltaT**Display → Cooler → *dT*

Here you can set the nominal difference with respect to ambient temperature.

Parameter range: -30 K...0 K

Factory setting: -15 K


Note: This menu will be hidden if the menu is locked.

**DeltaT mode**Display → Cooler → *Modu*


Here you can activate or deactivate DeltaT-mode.

Parameter range: *AbSo, dT*Factory setting: *AbSo* (normal operation mode)


Note: This menu will be hidden if the menu is locked.

**Exit submenu 1**Display → Submenu → *E*

Selecting this will return you to the main menu.

**5.4.4 Submenu 1 (global settings)****Temperature unit**Display → *LoP* → *uni t*

Used to select the temperature display unit.


Parameter range: *C, F*Factory setting: *C***Analog output**Display → *LoP* → *An 1*

This submenu is used to specify the settings for analog output 1, see chapter Submenu 2 (Analog Output 1)

Note: This menu will be hidden if the menu is locked.

## Calibrate moisture detector

Display → **LoP** → **h2o**



If a moisture detector is installed, calibration can now be performed. To do so, the unit must be flushed with dry gas.

Note:

Calibration was performed at the factory using ambient air. After replacing the moisture detector a calibration is again required.


Calibrating the moisture detector will set the menu **SEN** to **h1**.

This menu will be hidden if the menu is locked.

If the unit has multiple moisture detectors built in, they will be numbered in the menu. In this case, **h2o** indicates the first, **h2o2** the second moisture detector. The same applies to setting the sensor sensitivity in menu **SEN**.

## Moisture detector sensitivity

Display → **LoP** → **SEN**



If moisture detectors are installed, the sensitivity can be reduced here.

Parameter range:

**h1** : high sensitivity

**Lo**: low sensitivity

**non**: no moisture detector

Factory setting:

**h1**

Note:

This menu will be hidden if the menu is locked.

## Moisture detector: manual or automatic reset following moisture ingress

Display → **LoP** → **hLtc**

(**hLtc** = humidity latch). The setting applies to all connected moisture detectors.



Specifies whether the moisture ingress message must be reset manually or will automatically be reset after the sensor dries.

Parameter range:

**YES**: The status will be indicated until the user restarts the device and the pumps will be disabled.

**no**: The status message will automatically be cleared/the pumps will be released again once moisture is no longer detected.

Factory setting:

**no**

Note:

This menu will be hidden if the menu is locked.

## Moisture detector: error cleared automatically after cable break

Display → **LoP** → **bLtc**

(**bLtc** = broken wire latch). The setting applies to all connected moisture detectors.



Determines whether the cable break alarm must be reset manually or will automatically clear on valid measuring signal.

Parameter range:

**YES**: The status will be indicated until the user restarts the device. Clears the error, and the pumps will be deactivated.

**no**: The error message will disappear. The pumps will be switched on again once the moisture detector is reactivated again.

Factory setting:

**YES**


Note:

This menu will be hidden if the menu is locked.

## Lock Menu

To protect the menu from unauthorised use, enter a value for the lock code. Menu items can then only be accessed after entering the correct code.

Display → *LoP* → *Loc*



This setting will cancel/enable the menu lock.

Parameter range: 0 to 9999

Factory setting: 0 (keylock cancelled)

Note: This menu will be hidden if the menu is locked.

## Restart

Display → *LoP* → *rESt*

(*rESt* = restart)



The device will restart, all settings are saved. All error messages will be reset.  
The moisture detector will be reset, irrespective of the settings in menus *hi Lc* and *hilo*.

Parameter range: *yES*: Restart. The display will show the software version for the device and returns to measurement display.

*no*: Exit menu without restarting.

Note: The user settings will be saved.

## Factory settings

Display → *LoP* → *rSt*



This setting restores the factory settings.

Parameter range: *yES*: factory settings restored.

*no*: Exit menu without making changes.

Factory setting: *no*

Note: This menu will be hidden if the menu is locked.

## Exit submenu 1

Display → Submenu → *E*



Selecting this will return you to the main menu.

### 5.4.4.1 Submenu 2 (Analog Output 1)


The analog output will display the actual cooler temperature.

#### Signal behaviour

In normal mode (*noP*) the measuring point will output the actual temperature. For testing purposes you can generate constant values *hi*, *Lo* or *hRLF*. The analogue output will output a constant signal with a value as specified in the table.

Constant	Current output 4 – 20 mA	Voltage output 2 – 10 V
<i>hi</i>	20 mA	10 V
<i>fi</i>	12 mA	6 V
<i>Lo</i>	4 mA	2 V
<i>noP</i>	4 – 20 mA	2 – 10 V

After testing, the signal behaviour must be changed back to normal mode (*noP*).

Display → *LoP* → *Rn I* → *cout*

This setting determines how the analogue output will behave.

Parameter range: *noP* = Operation (normal mode), *hi*, *Lo*, *hRLF*Factory setting: *noP*

Note: This menu will be hidden if the menu is locked.

## Selection -> Output Signal

Display → *LoP* → *Rn I* → *out*

Select the type of output signal.

Parameter range: *,* Status output 4... 20 mA*v* Status output 2...10 VFactory setting: *,*Note: Disconnect meter before switching!  
This menu item is hidden if the keylock is enabled.

## Exit Submenu 2

Display → *LoP* → *Rn I* → *E*

Selecting this will return you to submenu 1.

## 5.4.5 Set favourite menu

Use the **F** or **Func** (function) key to set a favourite menu to later open it with just the push of a button.

- Open the menu you wish to set as the favourite. This menu can also be a lockable menu.
- Press the function key for more than 3 sec.  
The current menu has been set as the favourite. The display will briefly show the message *Func*.
- Press **ESC** or *E* (Exit) to return to the display.

To now access the favourite menu, press the **F** or **Func** key.**NOTICE! The favourite menu can also be accessed if the menu is locked.**

## 6 Maintenance

The base version of the cooler requires no special maintenance.

However, it may have different options depending on the cooler model. In this case the following routine maintenance is required:

- **Option peristaltic pump:** Checking hoses (see chapter Replacing the hoses of the peristaltic pump (option))
- **Filter option:** Checking the filter element (see chapter Replacing the filter element (option))
- **Option moisture detector:** Calibrating the moisture detector (see chapter Calibration of the moisture detector (option))
- **Option sample gas pump:** Checking valves for contamination. After 500 operating hours, tighten the screws for the mounting ring to 3 Nm. (see chapter Replacing sample gas pump inlet and outlet valves (optional))

During maintenance, remember:

- The equipment must be maintained by a professional familiar with the safety requirements and risks.
- Only perform maintenance work described in these operating and installation instructions.
- Observe the respective safety regulations and operating specifications when performing any type of maintenance.
- Always use genuine spare parts.
- For the option for high-purity water or oxygen, only use the explicitly designated replacement items with the suffix -H2 or -O2.

### DANGER

#### Electrical voltage

Electrocution hazard.



- Disconnect the device from power supply.
- Make sure that the equipment cannot be reconnected to mains unintentionally.
- The device must be opened by trained staff only.
- Regard correct mains voltage.



### DANGER

#### Toxic, corrosive gas/condensate

Sample gas/condensate may be hazardous to health.



- If necessary, ensure a safe gas/condensate discharge.
- Always disconnect the gas supply when performing maintenance or repairs.
- Protect yourself from toxic/corrosive gasses/condensate when performing maintenance. Wear appropriate protective equipment.



### CAUTION

#### Health hazard if the heat exchanger leaks

The heat exchanger is charged with glycol-based coolant.

In the event of a heat exchanger leak:



- Avoid contact with the skin and eyes.
- In the event of a leak, do not restart the cooler under any circumstances. The cooler must be repaired by the manufacturer.



## 7 Service and repair

This chapter contains information on troubleshooting and correction should an error occur during operation.

Repairs to the unit must be performed by Bühler authorised personnel.

Please contact our Service Department with any questions:

**Tel.: +49 (0) 2102-498955** or your agent

For more information on your custom maintenance and startup services, please visit: <https://www.buehler-technologies.com/service>

If the device is not functioning properly after correcting any malfunctions and switching on the power, it must be inspected by the manufacturer. Please send the equipment inside suitable packaging to:

**Bühler Technologies GmbH**

**- Reparatur/Service -**

**Harkortstraße 29**

**40880 Ratingen**

**Germany**

For devices for  $H_2/O_2$  applications, seal the gas and condensate path or return it without any parts in contact with the medium.

Please also attach the completed and signed RMA decontamination statement to the packaging. We will otherwise be unable to process your repair order.

You can find the form in the appendix of these instructions, or simply request it by e-mailing:

**[service@buehler-technologies.com](mailto:service@buehler-technologies.com)**.

### 7.1 Troubleshooting
















Problem / Malfunction	Possible cause	Action
Condensate inside the gas outlet	– Condensate trap full	– Empty condensate trap
	– Valve inside the automatic condensate drain may be stuck	– Flush in both directions
	– Cooler overloaded	– Maintain limits
Reduced gas flow rate	– Gas circuit clogged	– Uninstall and clean heat exchanger – if necessary, replace filter element
	– Condensate outlet iced over	– Send in unit
Excess temperature	– Operating point not yet reached	– Wait (max. 20 min)
	– Cooling outlet too long despite the cooler running	– Be sure the vents are not covered (heat buildup)
	– Flow rate / dew point / gas temperature too high	– Maintain limits / install pre-separator
	– Installed fan stopped	– Check and replace if necessary
Insufficient temperature	– Faulty control	– Send in cooler







## 7.1.1 Error messages on the display

If an error occurs, the display will read "Err". Press the "▲" button to show the error number(s).

Error messages will appear until the unit has been restarted or the error is cleared using the "Func" button. It can only be cleared if the cause for the error has been corrected.

**Causes / Action: The following is a list of the most common causes and actions for the respective error. If the actions listed do not resolve the problem, please contact Service.**

Problem/malfunction	Possible cause	Action
No display	<ul style="list-style-type: none"> <li>– No voltage</li> <li>– Loose connecting cable</li> <li>– Display failure</li> </ul>	<ul style="list-style-type: none"> <li>– Check the supply cable</li> <li>– Check fuse</li> <li>– Check connections</li> </ul>
 D1.02 (permanent)	(The software version for the display will appear). <ul style="list-style-type: none"> <li>– Not communicating with the controller</li> </ul>	<ul style="list-style-type: none"> <li>– Check connections</li> </ul>
 Error	<ul style="list-style-type: none"> <li>– An error has occurred</li> </ul>	<ul style="list-style-type: none"> <li>– Read the error number as described above</li> </ul>
 Error 01	<ul style="list-style-type: none"> <li>– Controller malfunction</li> </ul>	<ul style="list-style-type: none"> <li>– Clear error (temporary fault)</li> <li>– Disconnect from power for approx. 5 s</li> <li>– Contact service</li> </ul>
 Error 03	<ul style="list-style-type: none"> <li>– Microcontroller fault / MCP2</li> </ul>	<ul style="list-style-type: none"> <li>– Contact service</li> </ul>
 Error 04	<ul style="list-style-type: none"> <li>– EEPROM error</li> </ul>	<ul style="list-style-type: none"> <li>– Contact service</li> </ul>
 Error 22	<ul style="list-style-type: none"> <li>– Moisture detector 1 cable break</li> </ul>	<ul style="list-style-type: none"> <li>– Check moisture detector line</li> <li>– Check moisture detector</li> </ul>
 Error 32	<ul style="list-style-type: none"> <li>– Moisture detector 2 cable break</li> </ul>	<ul style="list-style-type: none"> <li>– Check moisture detector line</li> <li>– Check moisture detector</li> </ul>
 Error 40	<ul style="list-style-type: none"> <li>– General error temperature sensor 1 (block temperature)</li> </ul>	<ul style="list-style-type: none"> <li>– Possible sensor failure</li> </ul>
 Error 41	<ul style="list-style-type: none"> <li>– Low temperature / short-circuit temperature sensor 1</li> </ul>	<ul style="list-style-type: none"> <li>– Check temperature sensor connection</li> </ul>
 Error 42	<ul style="list-style-type: none"> <li>– Excess temperature / short-circuit temperature sensor 1</li> </ul>	<ul style="list-style-type: none"> <li>– Check temperature sensor connection</li> </ul>
 Error 43	<ul style="list-style-type: none"> <li>– Measurement fluctuation temperature sensor 1</li> </ul>	<ul style="list-style-type: none"> <li>– Check temperature sensor connection</li> </ul>
 Error 50	<ul style="list-style-type: none"> <li>– General error temperature sensor 2 (reference temperature Delta-T)</li> </ul>	<ul style="list-style-type: none"> <li>– Possible sensor failure</li> </ul>
 Error 51	<ul style="list-style-type: none"> <li>– Low temperature / short-circuit temperature sensor 2</li> </ul>	<ul style="list-style-type: none"> <li>– Check temperature sensor connection</li> </ul>
 Error 52	<ul style="list-style-type: none"> <li>– Excess temperature / short-circuit temperature sensor 2</li> </ul>	<ul style="list-style-type: none"> <li>– Check temperature sensor connection</li> </ul>
 Error 53	<ul style="list-style-type: none"> <li>– Measurement fluctuation temperature sensor 2</li> </ul>	<ul style="list-style-type: none"> <li>– Check temperature sensor connection</li> </ul>

Status text	Possible cause	Action
 H2o.1	– Moisture alarm moisture detector 1	– Dry – Check condensate trap
 H2o.2	– Moisture alarm moisture detector 2	– Dry – Check condensate trap
 init	– Initialisation phase	– Wait
 PuMP	– Pumps deactivated	– Reactive pumps via menu
 dt	Active Delta T control only: The block temperature is outside the defined temperature range. – Cooler is still in the "break-in phase" – Fluctuating ambient temperature – Insufficient cooling capacity	– Wait to see if the target temperature will be reached – Check the ambient temperature / power supplied – Process-related: Adjust alarm limits
 (Flashing)	– Excess/low temperature	– see chapter "Troubleshooting"

## 7.2 Safety instructions

- The device must be operated within its specifications.
- All repairs must be carried out by Bühler authorised personnel only.
- Only perform modifications, servicing or mounting described in this manual.
- Only use original spare parts.

**For sample gas coolers with stainless steel heat exchangers for O<sub>2</sub> applications (suffix -O2), there are special requirements for avoiding contamination when carrying out maintenance and repair work:**

Only use cleaned and undamaged tools. We recommend cleaning with a lint-free cloth, ideally pre-soaked with a mixture of isopropanol and demineralised water for residue-free degreasing.

Only use cleaned, original spare parts (see sections Spare Parts and Spare parts and accessories for cooler with -H2/-O2 heat exchanger).

Do not use any parts whose original packaging is damaged.

The use of compressed air is only permitted if it corresponds to at least class 2 in accordance with ISO 8573-1:2010.

### DANGER

#### Electrical voltage

Electrocution hazard.



- Disconnect the device from power supply.
- Make sure that the equipment cannot be reconnected to mains unintentionally.
- The device must be opened by trained staff only.
- Regard correct mains voltage.



### DANGER

#### Toxic, corrosive gas/condensate

Sample gas/condensate may be hazardous to health.



- If necessary, ensure a safe gas/condensate discharge.
- Always disconnect the gas supply when performing maintenance or repairs.
- Protect yourself from toxic/corrosive gasses/condensate when performing maintenance. Wear appropriate protective equipment.



**CAUTION****Health hazard if the heat exchanger leaks**

The heat exchanger is charged with glycol-based coolant.  
In the event of a heat exchanger leak:

- a) Avoid contact with the skin and eyes.
- b) In the event of a leak, do not restart the cooler under any circumstances. The cooler must be repaired by the manufacturer.

## 7.3 Cleaning and removal of the heat exchanger

Heat exchangers only need to be replaced or maintained if clogged or damaged. If they are clogged, we recommend checking whether using a filter will prevent this in future.

For applications with high-purity acid or hydrogen, we recommend cleaning in accordance with current application-specific standards or using an original replacement heat exchanger.

- Close gas supply.
- Switch off device and disconnect all plugs (e.g. status output connector, supply input, etc.).
- Disconnect gas connections and condensate drain.
- Pull the heat exchanger up and out.
- Clean cleaning nest (hole inside the cooler block), as the heat exchangers are installed with silicone grease.
- Purge the heat exchanger until all contaminants have been removed.
- Lubricate the cooled external surface with silicone grease.
- Reinsert the heat exchanger into the cooling nest with a rotating motion.
- Reconnect the gas supply and condensate drain. The gas inlet is marked red.
- Restore power/gas supply and wait until the unit is ready for operation.
- Open gas supply.

## 7.4 Replacing the hoses of the peristaltic pump (option)

- Close gas supply.
- Switch off device and disconnect all plugs (e.g. connector plug status output, supply input, etc.).
- Disconnect supply and discharge tube on peristaltic pump (**observe safety notes!**).
- Loosen but do not remove centre knurled nut. Flip down the screw.
- Pull cover up and off.
- Unplug external connections and remove hose.
- Replace hose (Bühler spare part) and install peristaltic pump in reverse order.
- Restore the power and gas supply.

## 7.5 Replacing the filter element (option)

**CAUTION****Gas leakage**

The filter should not be dismantled under pressure.  
Don't use damaged parts again.

- Close the gas supply.
- Switch off and unplug the device.
- Pull the bracket, holding on to the filter glass.
- Whilst holding the filter head, move the glass back and forth and carefully remove downward.
- Remove the filter element and insert a new one.
- Check for leaks and replace, if necessary.
- Whilst holding the filter head, move the glass back and forth and carefully reattach the filter head, attach the bracket, and ensure it is seated securely.
- Restore the power and gas supply.

**NOTICE!** Please observe legal regulations when disposing of filter elements.


## 7.6 Drying of the moisture detector (option)

The moisture detector must be dried if moisture enters.

- Close the gas supply.
- Switch off and unplug the device.
- Loosen the swivel nut for the moisture detector connection line and disconnect the line.
- Unscrew the moisture detector counter-clockwise and remove.
- Dry moisture detector.
- Reinsert the moisture detector and carefully tighten the screw connection.
- Connect the connection line and tighten the swivel nut.
- Restore the power and gas supply.

## 7.7 Calibration of the moisture detector (option)

- When replacing the moisture detectors, they must be recalibrated.
- Be sure dry gas flows through the cooler.
- Select cooler menu and confirm.





- Select menu item moisture detector.



- The display shows (Reset).
- Confirm the display to calibrate the moisture detectors.

**For a detailed overview of menu navigation, refer to chapter "Operation and Control".**

## 7.8 Replacing sample gas pump inlet and outlet valves (optional)

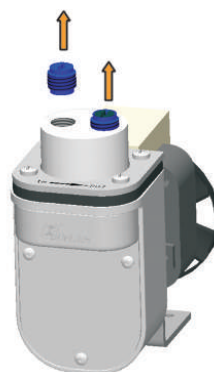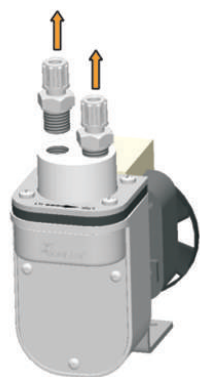

First detach the screw connections.


Unscrew the inlet or outlet valve with a wide slot screwdriver.

**Attention:** The PVDF and PVDF with bypass valve pump bodies already have PTFE gaskets installed in the gas inlets and outlets. These are also included in the valve spare parts kit. Remove the old gaskets before installing the new ones.

The inlet and outlet valves are identical. Their installation position determines the function. As shown in the image, the valves are blue on one side and black on the other. The valves are further marked "IN" or for inlet and "OUT" for outlet.

Inlet valve

Outlet valve




To assemble the sample gas pump, perform the steps in reverse order. When tightening the inlet and outlet valves be sure to observe the required tightening torque of max. 1 Nm. **CAUTION! Tightening the valves more will permanently deform the pump body, requiring replacement.**



When installing the screw connection, ensure the connection is tight.

## 7.9 Replacing the O-ring on the bypass valve (optional)

- Loosen the two screws on the valve plate and carefully remove the entire unit.
- Coat the new O-ring with suitable O-ring grease (min. operating temperature 145 °C, e.g. Fluoronox S90/2) and install in the spindle.
- Carefully insert the entire unit into the pump body while turning and tighten screws.

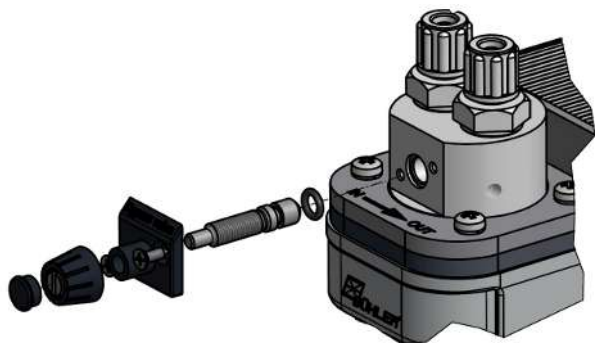

## 7.10 Replacing the bellow (optional)

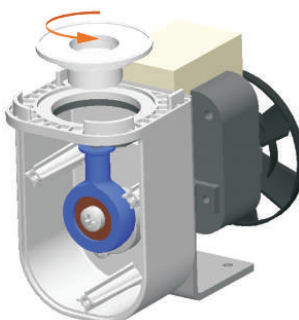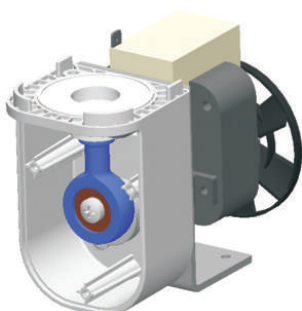

To replace the bellow carefully unscrew it from the connecting rod counter clockwise. Be sure not to lose any installed shims.

Before reinstalling the bellow be sure it is not damaged.

Reinstall hand tight in reverse order.

## 7.11 Spare Parts

Please also specify the model and serial number when ordering parts.

Upgrade and expansion parts can be found in our catalog.

Available spare parts:

Item no.	Description
9100100007	Display module MCD400
9144050079	Connecting cable controller board display module
9100130380	Microcontroller board MCP2.2
4011000	Flow adapter type G, PVDF G1/4
40110001	Flow adapter type NPT, PVDF NPT 1/4"
4011005	Flow adapter type G, stainless steel, G1/4
40110051	Flow adapter type NPT, stainless steel, NPT 1/4"
4111100	Moisture detector FF-3-N, without cable
9144050081	Moisture detector connection cable, 300 mm
9144050086	Moisture detector connection cable, 520 mm
4150799	Filter AGF-PV-30-F2-L, G1/4
41507991	Filter AGF-PV-30-F2-L, NPT 1/4"
9100010198	Power board
9100011187	Controller board
see data sheet 420013	Sample Gas Pumps P1.3
see data sheet 450022	Peristaltic Pumps CPsingle, CPdouble X2

### 7.11.1 Consumables and accessories

Item no.	Description
4510008	Automatic condensate drain AK 5.2 (pressure operation only)
4510028	Automatic condensate drain AK 5.5 (pressure operation only)
4410004	Automatic condensate drain AK 20 (pressure operation only)
4410001	Automatic condensate drain 11 LD V 38 (pressure operation only)
9144050038	Cable for cooler temperature analog output 4 m
41020050	Filter element F2-L; 2-pack
4410005	Condensate trap GL1, 0.4 L
44920035012	Condensate pump replacement hose, Tygon (Norprene), angled hose nipple
44920035016	Condensate pump replacement hose, Tygon (Norprene), angled hose nipple and screw connection (metric)
44920035017	Condensate pump replacement hose, Tygon (Norprene), angled hose nipple and screw connection (US)
4228003	Bellow for P1 pump
9009398	O-ring for bypass P1 pump
4228066	Set inlet/outlet valves 70 °C for P1 pump
see data sheet 420011	Sample Gas Pumps P1
see data sheet 450020	CPsingle, CPdouble peristaltic condensate pumps

### 7.11.2 Spare parts and accessories for cooler with -H2/-O2 heat exchanger

Item no.	Description
4410001 (see data sheet 450005)	Automatic condensate drain 11 LD V 38 <sup>1)</sup>
4410001-O2 (see data sheet 450005)	Automatic condensate drain 11 LD V 38 optimised for oxygen
see data sheet 400016	Stainless steel pipe fittings for high-purity oxygen applications

<sup>1)</sup> For use with high hydrogen concentrations max. 1.5 bar overpressure.

## 8 Disposal

The heat exchanger is charged with glycol-based coolant.

The applicable national laws must be observed when disposing of the products. Disposal must not result in a danger to health and environment.

The crossed out wheelie bin symbol on Bühler Technologies GmbH electrical and electronic products indicates special disposal notices within the European Union (EU).



The crossed out wheelie bin symbol indicates the electric and electronic products bearing the symbol must be disposed of separate from household waste. They must be properly disposed of as waste electrical and electronic equipment.

Bühler Technologies GmbH will gladly dispose of your device bearing this mark. Please send your device to the address below for this purpose.



We are obligated by law to protect our employees from hazards posed by contaminated devices. Therefore please understand that we can only dispose of your waste equipment if the device is free from any aggressive, corrosive or other operating fluids dangerous to health or environment. **Please complete the "RMA Form and Decontamination Statement", available on our website, for every waste electrical and electronic equipment. The form must be applied to the packaging so it is visible from the outside.**

Please return waste electrical and electronic equipment to the following address:

Bühler Technologies GmbH  
WEEE  
Harkortstr. 29  
40880 Ratingen  
Germany

Please also observe data protection regulations and remember you are personally responsible for the returned waste equipment not bearing any personal data. Therefore please be sure to delete your personal data before returning your waste equipment.



## 9 Appendices

### 9.1 Gas cooler technical data

#### TC-MIDI X2

Gas Cooler Technical Data				
Ready for operation	after max. 10 minutes			
Ambient temperature	5 °C to 60 °C			
Gas output dew temperature preset:	5 °C			
adjustable:	2 °C...20 °C or Delta T control			
IP rating	IP 20			
Mechanical load	Tested based on DNV-GL CG0339 vibration class A (0.7g) <sup>1)</sup> 2 Hz-13.2 Hz amplitude ± 1.0 mm 13.2 Hz -100 Hz acceleration			
Housing	Stainless steel, brushed			
Packaging dimensions	approx. 350 x 220 x 220 mm			
Weight incl. heat exchanger	approx. 11.5 kg approx. 15 kg at full expansion stage			
Electrical data	Unit without add-on		Unit with add-on (P1.x + peristaltic pump)	
	<b>230 V AC</b>	<b>115 V AC</b>	<b>230 V AC</b>	<b>115 V AC</b>
	+5/-10%	+5/-10%	+/-5%	+/-5%
	50/60 Hz	50/60 Hz	50 Hz	60 Hz
	1.2 A	2.4 A	1.8 A	3.6 A
	200 W / 280 VA		290 W / 420 VA	
Recommended fuse (characteristic: delayed action)	3.15 A	6.3 A	3.15 A	6.3 A
Status output switching capacity	max. 250 V AC, 150 V DC 2 A, 50 VA, potential-free			
Electrical Connections	Plug per EN 175301-803			
Gas connections and condensate outlet	Heat exchanger see table "Heat Exchanger Overview" Filter, moisture detector adapter G1/4 or NPT 1/4"			
Parts in contact with media				
Filter:	see "Technical Data - Options"			
Moisture detector:	see "Technical Data - Options"			
Heat exchanger:	see table "Heat Exchanger Overview"			
Peristaltic pump:	see "Technical Data - Options"			
Sample gas pump:	see "Technical Data - Options"			
Tubing:	PTFE/Viton			
Markings:	FM18ATEX0012X: II 3 G Ex ec nC IIC T4 Gc IECEx FMG 18.0005X: Ex ec nC IIC T4 Gc FM18US0021X/FM18CA0010X: CL I DIV 2 GP ABCD RU C-DE.HA65.B.00608/20			

<sup>1)</sup> not in conjunction with add-on sample gas pump

## TC-MIDI X2 with -H2/-O2 heat exchanger

## Gas Cooler Technical Data

Ready for operation	after max. 10 minutes	
Ambient temperature	5 °C to 60 °C	
Gas outlet dew point preset:	5 °C	
adjustable:	2 °C...20 °C	
IP rating	IP 20	
Mechanical load	Tested based on DNV-GL CG0339 vibration class A (0.7 g) 2–13.2 Hz amplitude ± 1.0 mm 13.2–100 Hz acceleration	
Housing	Stainless steel, brushed	
Packaging dimensions	approx. 350 x 220 x 220 mm	
Weight incl. heat exchanger	approx. 12 kg	
Electrical data	Unit without add-on	
	<b>230 V AC</b>	<b>115 V AC</b>
	+5/-10%	+5/-10%
	50/60 Hz	50/60 Hz
	1.2 A	2.4 A
	200 W / 280 VA	
Recommended fuse (characteristic: delayed action)	3.15 A	6.3 A
Status output switching capacity	max. 250 V AC, 150 V DC 2 A, 50 VA, potential-free	
Electrical Connections	Plug per EN 175301-803	
Parts in contact with media Heat exchanger:	see table "Heat Exchanger Overview"	
Markings:	FM18ATEX0012X: II 3 G Ex ec nC IIC T4 Gc IECEX FMG 18.0005X: Ex ec nC IIC T4 Gc FM18US0021X/FM18CA0010X: CL I DIV 2 GP ABCD RU C-DE.HA65.B.00608/20	

## TC-MIDI+ X2

## Gas Cooler Technical Data

Ready for operation	after max. 10 minutes			
Ambient temperature	5 °C to 60 °C			
Gas output dew temperature preset:	5 °C			
adjustable:	2 °C...20 °C			
IP rating	IP 20			
Mechanical load	Tested based on DNV-GL CG0339 vibration class A (0.7g) <sup>1)</sup> 2 Hz-13.2 Hz amplitude ± 1.0 mm 13.2 Hz -100 Hz acceleration			
Housing	Stainless steel, brushed			
Packaging dimensions	approx. 350 x 220 x 220 mm			
Weight incl. heat exchanger	approx. 12 kg approx. 15.5 kg at full expansion stage			
Electrical data	Unit without add-on		Unit with add-on (P1.x + peristaltic pump)	
	<b>230 V AC</b>	<b>115 V AC</b>	<b>230 V AC</b>	<b>115 V AC</b>
	+5/-10%	+5/-10%	+/-5%	+/-5%
	50/60 Hz	50/60 Hz	50 Hz	60 Hz
	1.2 A	2.4 A	1.8 A	3.6 A
	200 W / 280 VA		290 W / 420 VA	
Recommended fuse (characteristic: delayed action)	3.15 A	6.3 A	3.15 A	6.3 A
Status output switching capacity	max. 250 V AC, 150 V DC 2 A, 50 VA, potential-free			
Electrical Connections	Plug per EN 175301-803			
Gas connections and condensate outlet	Heat exchanger see table "Heat Exchanger Overview" Filter, moisture detector adapter G1/4 or NPT 1/4"			
Parts in contact with media				
Filter:	see "Technical Data - Options"			
Moisture detector:	see "Technical Data - Options"			
Heat exchanger:	see table "Heat Exchanger Overview"			
Peristaltic pump:	see "Technical Data - Options"			
Sample gas pump:	see "Technical Data - Options"			
Tubing:	PTFE/Viton			
Markings:	FM18ATEX0012X: II 3 G Ex ec nC IIC T4 Gc IECEx FMG 18.0005X: Ex ec nC IIC T4 Gc FM18US0021X/FM18CA0010X: CL I DIV 2 GP ABCD RU C-DE.HA65.B.00608/20			

<sup>1)</sup> not in conjunction with add-on sample gas pump

## 9.2 Technical Data - Options

### Analogue Output Cooler Temperature Technical Data

Signal	4-20 mA or 2-10 V corresponds to -20 °C to +60 °C cooler temperature
Connection	M12x1 plug, DIN EN 61076-2-101

### Technical Data peristaltic pumps CPsingle X2 / CPdouble X2

Ambient temperature	0 °C to 50 °C
Flow rate	0.3 L/h (50 Hz) / 0.36 L/h (60 Hz) with standard hose
Vacuum inlet	max. 0.8 bar
Pressure inlet	max. 1 bar
Outlet pressure	1 bar
Hose	4 x 1.6 mm
Condensate outlet	Hose nipple Ø6 mm Screw connection 4/6 (metric), 1/6"-1/4" (US)
Protection class	IP 40
Materials	
Hose:	Norprene (Standard), Marprene, Fluran
Connections:	PVDF

### Technical Data Sample Gas Pump P1.3

Ambient temperature	0 °C to 50 °C
Operating pressure	max. 1,3 bar abs.
Nominal outlet	280 l/h (at p = 1 bar abs.)
Materials in contact with media vary by configuration	PTFE, PVDF, 1.4571, 1.4401, Viton

### Technical Data Filter AGF-PV-30-F2-L

Ambient temperature	3 °C to 100 °C
max. operating pressure with filter	4 bar
Filter surface	125 cm <sup>2</sup>
Filter fineness	2 µm
Dead volume	108 ml
Materials	
Filter:	PVDF, Duran glass (parts in contact with mediums)
Seal:	Viton
Filter element:	sintered PTFE


### Technical Data FF-3-N Moisture Detector

Ambient temperature	3 °C to 50 °C
max. operating pressure with FF-3-N	2 bar
Material	PVDF, PTFE, epoxy resin, stainless steel 1.4571, 1.4576

## 9.3 Flow diagrams

### TC-MIDI


Standard hoses each gas path

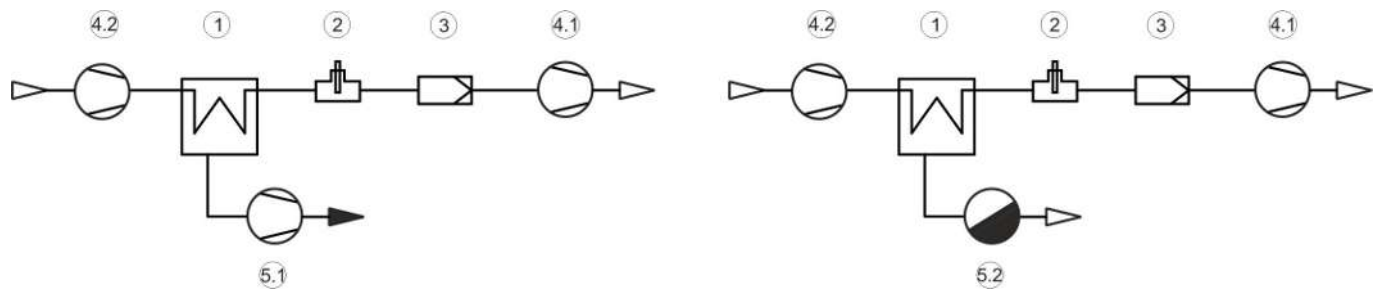

1 Cooler	4.2 Sample Gas Pump, Pressure Operation (Optional)
2 Moisture detector (optional)	5.1 Condensate pump (optional)
3 Filter (optional)	5.2 Automatic Condensate Drain, Pressure Operation (Optional)
4.1 Sample Gas Pump, Suction Operation (Optional)	

### TC-MIDI+


1 gas path in series

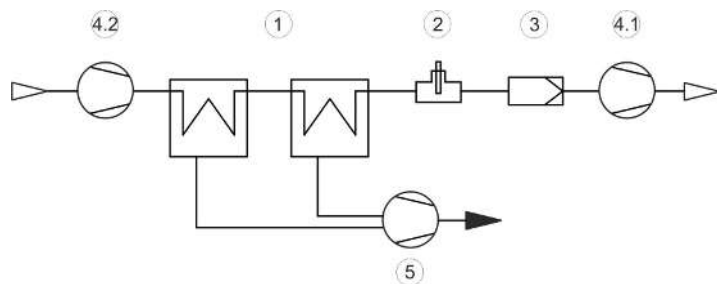

1 Cooler	4.1 Sample Gas Pump, Suction Operation (Optional)
2 Moisture detector (optional)	4.2 Sample Gas Pump, Pressure Operation (Optional)
3 Filter (optional)	5 Condensate pump (optional)


## 9.4 Performance data

### TC-MIDI

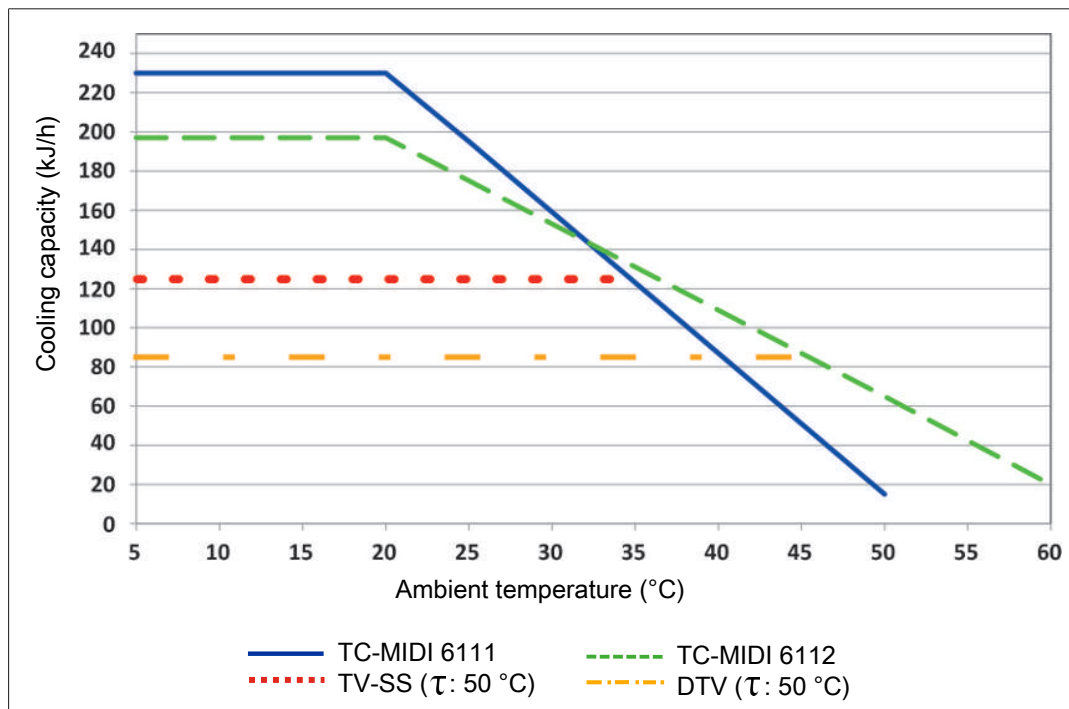


Note: The limit curves for the heat exchangers apply to a dew point of 50 °C.

### TC-MIDI with -H2/-O2 heat exchanger

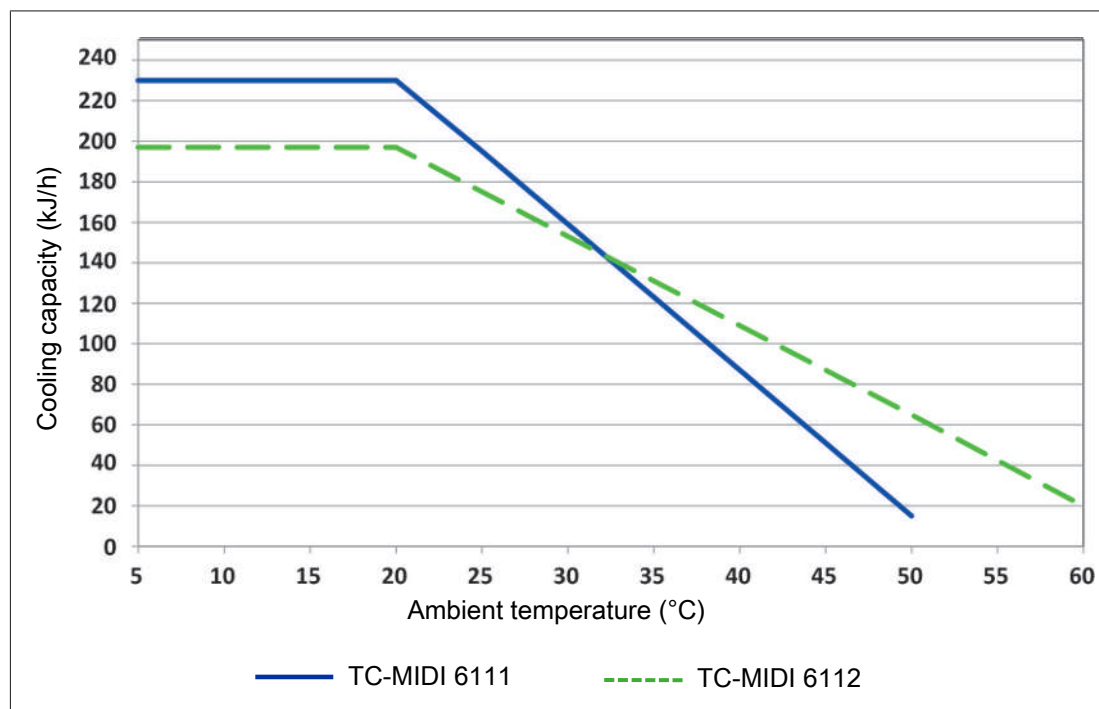

Note: The limit curves for the heat exchangers apply to a dew point of 50 °C.

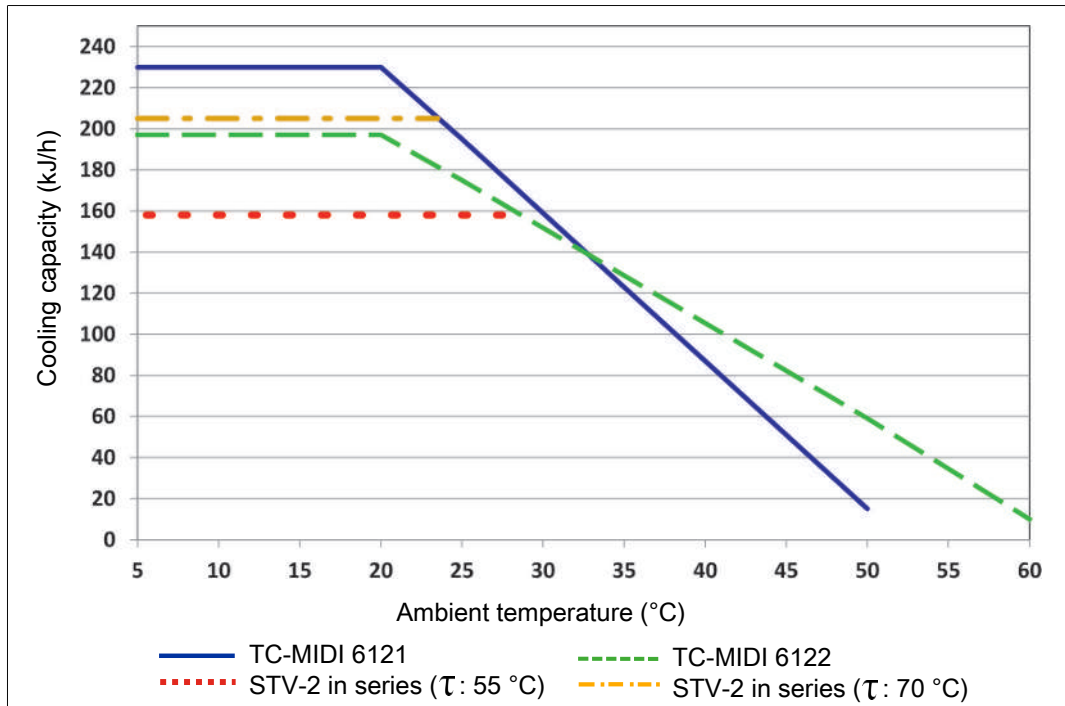**TC-MIDI+**

Note: The capacity of STG-2 heat exchangers is equivalent to the maximum cooling capacity of the cooler.

## 9.5 Heat exchanger

### 9.5.1 Heat exchanger description

#### TC-MIDI

The energy content of the sample gas and the required cooling capacity of the gas cooler is determined by three parameters: gas temperature  $\vartheta_G$ , dew point  $\tau_e$  (moisture content) and volume flow  $v$ . The outlet dew point rises with increasing energy content of the gas. The approved energy load from the gas is therefore determined by the tolerated rise in the dew point.

The following limits are specified for a standard operating point of  $\tau_e = 50^\circ\text{C}$  and  $\vartheta_G = 70^\circ\text{C}$ . The maximum volume flow  $v_{\max}$  in  $\text{NI/h}$  of cooled air is indicated, so after moisture has condensed.

If the values fall below  $\tau_e$  and  $\vartheta_G$ , the flow  $v_{\max}$  may be increased. For example, on the TG heat exchanger the parameter triple  $\tau_e = 40^\circ\text{C}$ ,  $\vartheta_G = 70^\circ\text{C}$  and  $v = 425 \text{ NI/h}$  may also be used in place of  $\tau_e = 50^\circ\text{C}$ ,  $\vartheta_G = 70^\circ\text{C}$  and  $v = 345 \text{ NI/h}$ .

Please contact our experts for clarification or refer to our design program.

#### TC-MIDI+

The energy content of the sample gas and the required cooling capacity of the gas cooler is determined by three parameters: gas temperature  $\vartheta_G$ , dew point  $\tau_e$  (moisture content) and volume flow  $v$ . The outlet dew point rises with increasing energy content of the gas. The approved energy load from the gas is therefore determined by the tolerated rise in the dew point.

The following limits are specified for a standard operating point of  $\tau_e = 50^\circ\text{C}$  and  $\vartheta_G = 70^\circ\text{C}$ . The maximum volume flow  $v_{\max}$  in  $\text{NI/h}$  of cooled air is indicated, so after moisture has condensed.

If the values fall below  $\tau_e$  and  $\vartheta_G$ , the flow  $v_{\max}$  may be increased. For example, on the STG-2 heat exchanger the parameter triple  $\tau_e = 40^\circ\text{C}$ ,  $\vartheta_G = 70^\circ\text{C}$  and  $v = 575 \text{ NI/h}$  may also be used in place of  $\tau_e = 50^\circ\text{C}$ ,  $\vartheta_G = 70^\circ\text{C}$  and  $v = 320 \text{ NI/h}$ .

Please contact our experts for clarification or refer to our design program.

## 9.5.2 Heat exchanger overview

### TC-MIDI

Heat exchanger	TS TS-I <sup>2)</sup>	TG TG-I <sup>2)</sup>	TV TV-I <sup>2)</sup>	DTS (DTS-6 <sup>3)</sup> ) DTS-I (DTS-6-I <sup>3)</sup> ) <sup>2)</sup>	DTG DTG-I <sup>2)</sup>	DTV <sup>3)</sup> DTV-I <sup>2) 3)</sup>
Materials in contact with media	Stainless steel	Glass PTFE	PVDF	Stainless steel	Glass PTFE	PVDF
Flow rate $v_{\max}$ <sup>1)</sup>	500 L/h	400 L/h	235 L/h	2 x 250 L/h	2 x 200 L/h	2 x 160 L/h
Inlet dew point $\tau_{e,\max}$ <sup>1)</sup>	80 °C	80 °C	65 °C	80 °C	65 °C	65 °C
Gas inlet temperature $\vartheta_{G,\max}$ <sup>1)</sup>	180 °C	140 °C	140 °C	180 °C	140 °C	140 °C
Max. cooling capacity $Q_{\max}$	450 kJ/h	230 kJ/h	120 kJ/h	450 kJ/h	230 kJ/h	185 kJ/h
Gas pressure $p_{\max}$	160 bar	3 bar	3 bar	25 bar	3 bar	2 bar
Pressure drop $\Delta p$ ( $v=150$ L/h)	8 mbar	8 mbar	8 mbar	5 mbar each	5 mbar each	15 mbar each
Dead volume $V_{\text{tot}}$	69 ml	48 ml	129 ml	28 / 25 ml	28 / 25 ml	21 / 21 ml
Gas connections (metric)	G1/4	GL 14 (6 mm) <sup>4)</sup>	DN 4/6	6 mm tube	GL14 (6 mm) <sup>4)</sup>	DN 4/6
Gas connections (US)	NPT 1/4"	GL 14 (1/4") <sup>4)</sup>	1/4"-1/6"	1/4" tube	GL14 (1/4") <sup>4)</sup>	1/4"-1/6"
Condensate out connections (metric)	G3/8	GL 25 (12 mm) <sup>4)</sup>	G3/8	Tube 10 mm (6 mm)	GL18 (10 mm) <sup>4)</sup>	DN 5/8
Condensate out connections (US)	NPT 3/8"	GL 25 (1/2") <sup>4)</sup>	NPT 3/8"	Tube 3/8" (1/4")	GL18 (3/8") <sup>4)</sup>	3/16"-5/16"

<sup>1)</sup> Max. cooling capacity of the cooler must be considered.

<sup>2)</sup> Models marked I have NPT threads or US tubes, respectively.

<sup>3)</sup> Condensate drain only possible with condensate pump.

<sup>4)</sup> Gasket inside diameter.

### TC-MIDI with -H2/-O2 heat exchanger

Heat exchanger	TS-H2/-O2 TS-I-H2/-O2 <sup>2)</sup>	DTS-H2/-O2 DTS-I-H2/-O2 <sup>2)</sup>
Materials in contact with media	Stainless steel	Stainless steel
Flow rate $v_{\max}$ <sup>1)</sup>	500 l/h	2x 250 l/h
Inlet dew point $\tau_{e,\max}$ <sup>1)</sup>	80 °C	80 °C
Gas inlet temperature $\vartheta_{G,\max}$ <sup>1)</sup>	180 °C	180 °C
Max. cooling capacity $Q_{\max}$	450 kJ/h	450 kJ/h
Gas pressure $p_{\max}$	1.5 bar	1.5 bar
Pressure drop $\Delta p$ ( $v=150$ l/h)	8 mbar	5 mbar each
Dead volume $V_{\text{dead}}$	69 ml	28/25 ml
Gas connections (metric)	G1/4	6 mm tube
Gas connections (US)	NPT 1/4"	1/4" tube
Condensate out connection (metric)	G3/8	Tube 10 mm (6 mm)
Condensate out connection (US)	NPT 3/8"	Tube 3/8" (1/4")

<sup>1)</sup> Max. cooling capacity of the cooler must be considered.

<sup>2)</sup> Models marked I have NPT threads or US tubes.



**TC-MIDI+**

Heat exchanger	2x STG-2 2x STG-2-I <sup>2)</sup>	2x STV-2 2x STV-2-I <sup>2)</sup>
Materials in contact with media	Glass PTFE	PVDF
Flow rate $v_{\max}$ <sup>1)</sup>	320 L/h	300 L/h
Inlet dew point $\tau_{e,\max}$ <sup>1)</sup>	70 °C	70 °C
Gas inlet temperature $\vartheta_{G,\max}$ <sup>1)</sup>	140 °C	140 °C
Gas pressure $p_{\max}$	3 bar	3 bar
Pressure drop $\Delta p$ ( $v=150$ L/h)	2.6 mbar	2.9 mbar
Max. Cooling capacity $Q_{\max}$	345 kJ/h	210 kJ/h
Dead volume $V_{\text{tot}}$	47 ml	41 ml
Gas connections (metric)	GL 14 (6 mm) <sup>3)</sup>	DN 4/6
Gas connections (US)	GL 14 (1/4") <sup>3)</sup>	1/4"-1/6"
Condensate out connection (metric)	GL 18 (10 mm) <sup>3)</sup>	G1/4
Condensate out connection (US)	GL18 (10 mm) <sup>3)</sup>	NPT 1/4"


<sup>1)</sup> Max. cooling capacity of the cooler must be considered.

<sup>2)</sup> Models marked I have NPT threads or US tubes, respectively.


<sup>3)</sup> Gasket inside diameter

## 9.6 Dimensions (mm)


### TC-MIDI

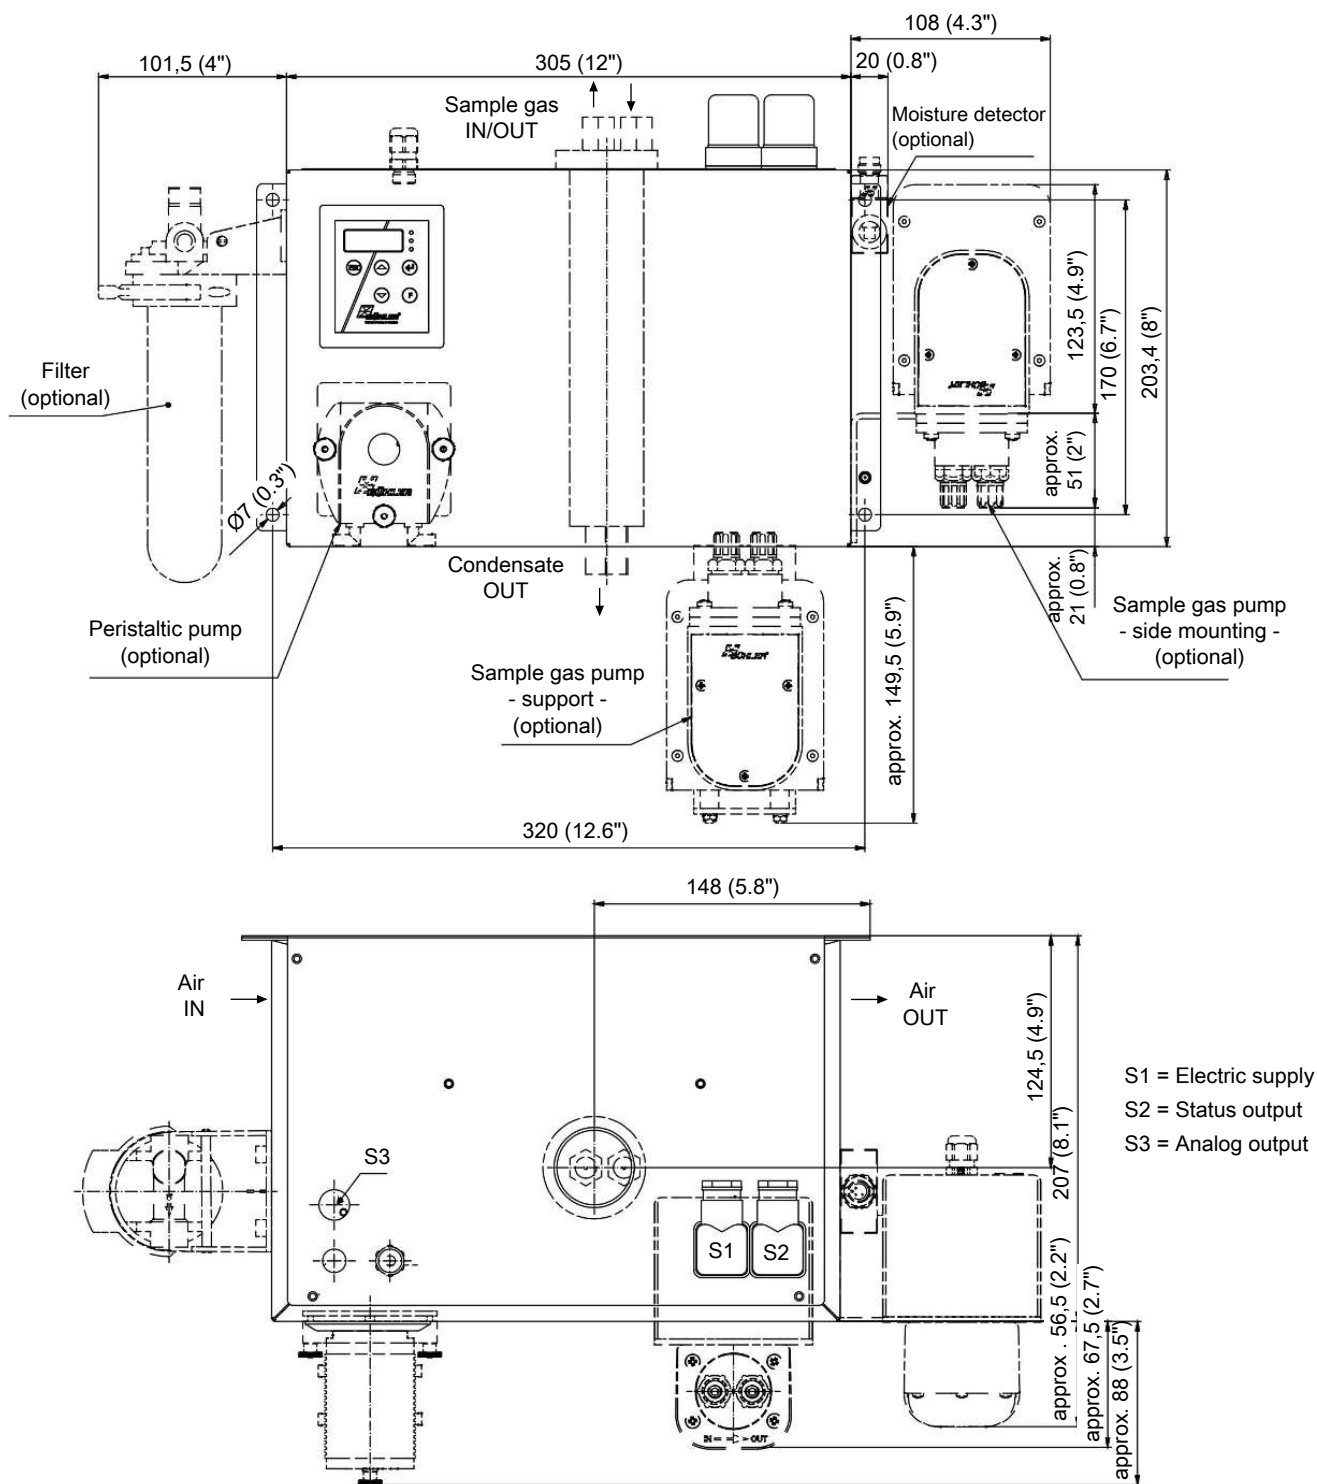

# TC-MIDI with -H2/-O2 heat exchanger

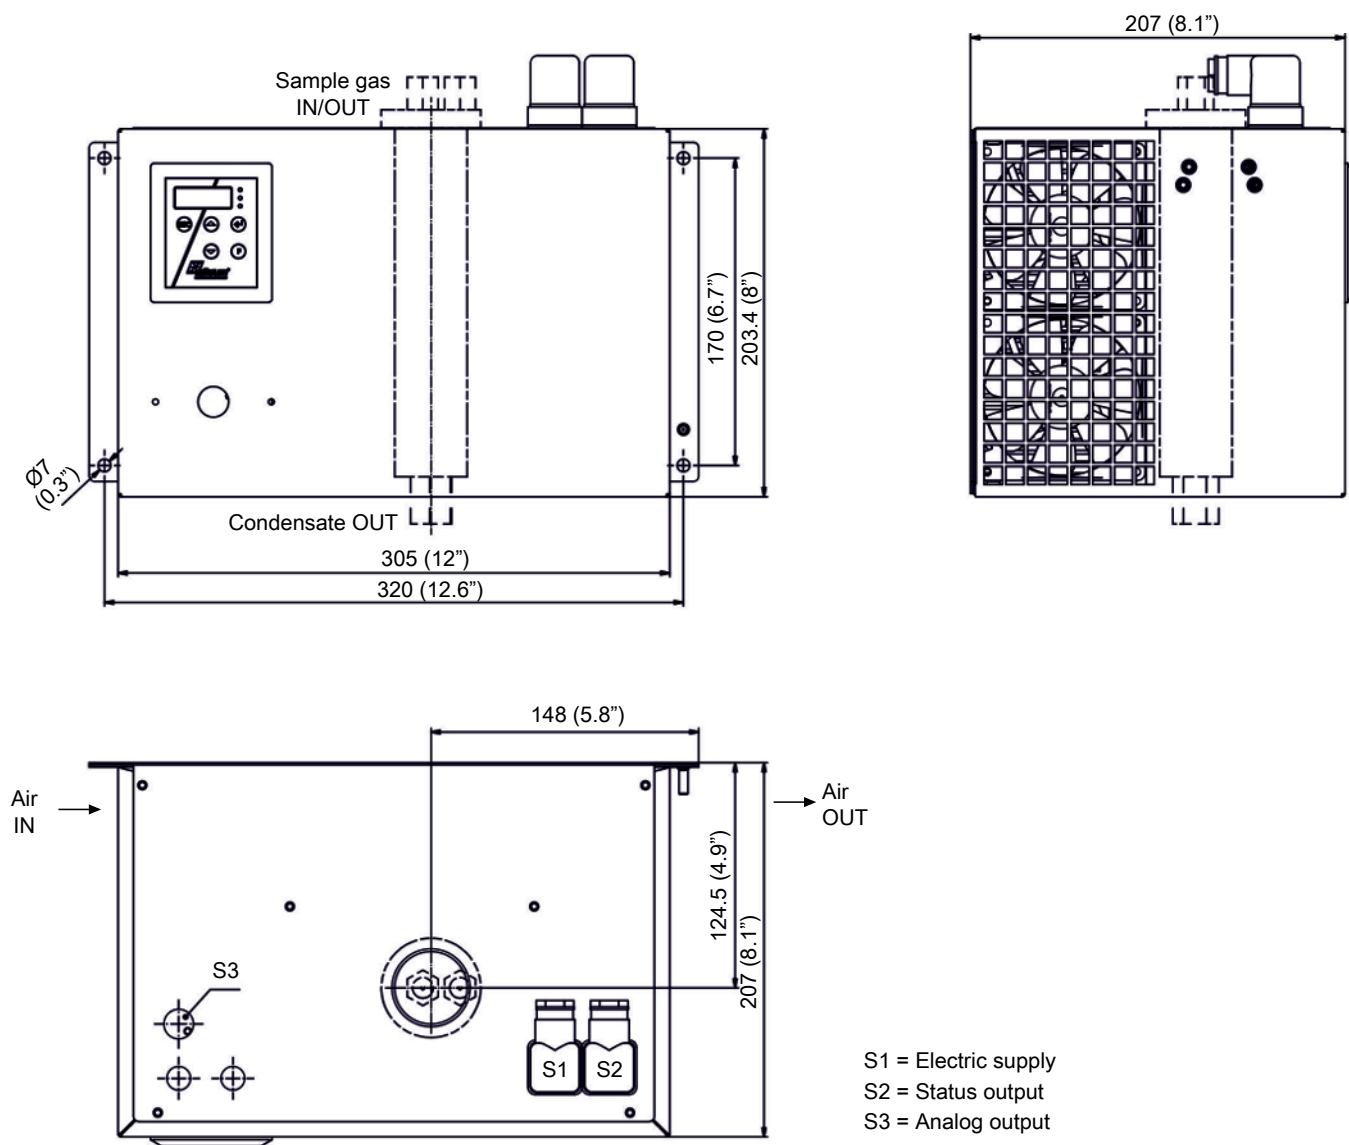

TC-MIDI+

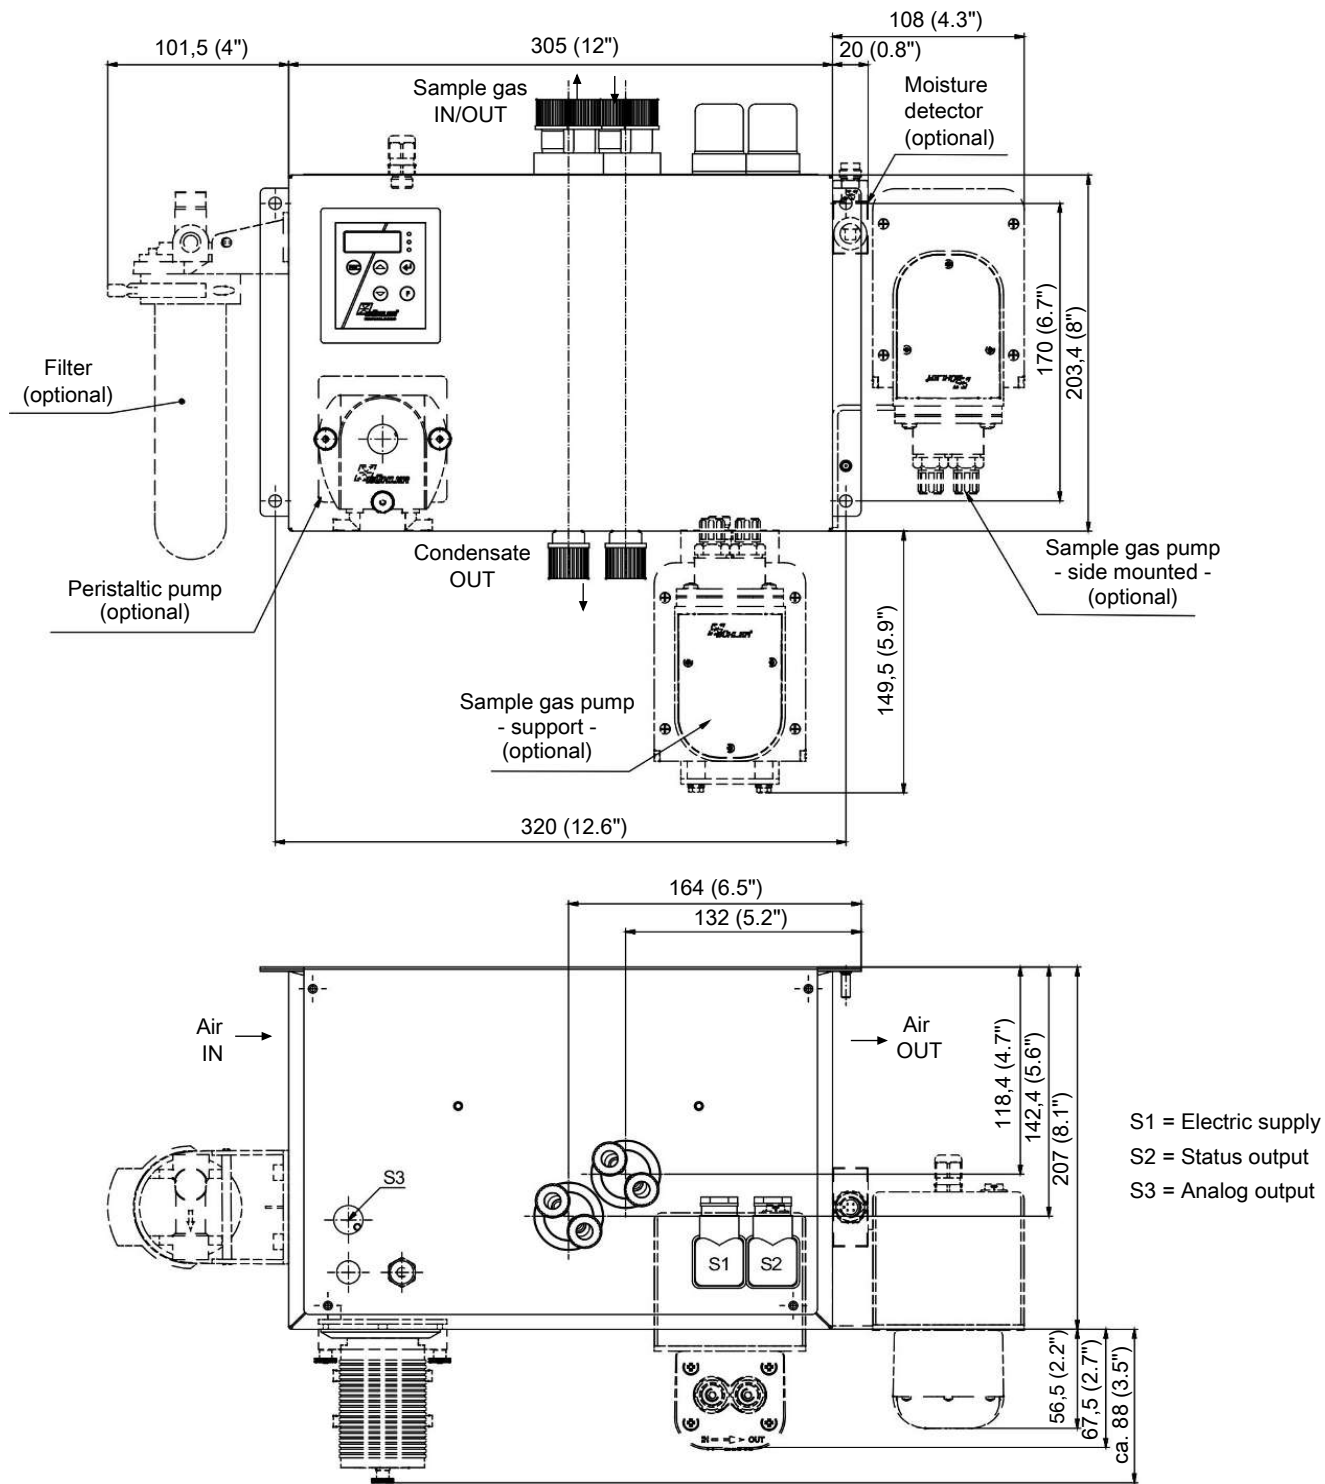

## **10 Attached documents**

- Declaration of Conformity
- O<sub>2</sub> declaration (heat exchanger)
- Certificates
- RMA – Decontamination Statement

## EU-Konformitätserklärung EU-declaration of conformity



Hiermit erklärt Bühler Technologies GmbH, dass die nachfolgenden Produkte den wesentlichen Anforderungen der Richtlinie

Herewith declares Bühler Technologies GmbH that the following products correspond to the essential requirements of Directive

2014/34/EU  
(Atex)


in ihrer aktuellen Fassung entsprechen.

in its actual version.

**Produkt / products:** Messgaskühler / Sample gas cooler  
**Typ / type:** TC-Standard X2, TC-MIDI X2, TC-Double X2  
TC-Standard+ X2, TC-MIDI+ X2, TC-Double+ X2

Die Produkte werden entsprechend der derzeit gültigen Atex-Richtlinie innerhalb der internen Fertigungskontrolle folgendermaßen gekennzeichnet:

*The products are marked according to the currently valid Atex directive during internal control of production:*

**Atex:**  II 3 G Ex ec nC IIC T4 Gc  
**IECEx:** Ex ec nC IIC T4 Gc

Die Eignung dieses Produkts für die Zone 2 wurde durch eine Baumusterprüfbescheinigung mit der Nummer FM18ATEX0012X festgestellt.

Die Betriebsanleitung zu diesem Produkt beinhaltet besondere Installations- und Betriebsbedingungen und sind für die sichere Anwendung zu beachten.

*This product's suitability for Zone 2 was determined by type-examination certificate number FM18ATEX0012X.*

*The operating instructions for this product contains special installation and operating conditions and must be observed to ensure safe operation.*

Zur Beurteilung der Konformität wurden folgende harmonisierte Normen herangezogen:  
*For the assessment of conformity the following standards have been used:*

**EN 60079-0:2012 + A11:2013**

**EN 60079-7:2015+A1:2018**

**EN 60079-15:2018**

Der Hersteller hat die Übereinstimmung des Gerätes mit aktuelleren Normenausgaben als in der Baumusterprüfbescheinigung aufgeführt geprüft und die Konformität festgestellt:

*The manufacturer has checked the compliance of the device with more current standards than those listed in the type examination certificate and has established conformity:*

**EN IEC 60079-0:2018**

**EN IEC 60079-7:2015 + A1:2018**

Dokumentationsverantwortlicher für diese Konformitätserklärung ist Herr Stefan Eschweiler mit Anschrift am Firmensitz.

*The person authorised to compile the technical file is Mr. Stefan Eschweiler located at the company's address.*

Ratingen, den 01.03.2021

  
Stefan Eschweiler  
Geschäftsführer – Managing Director

  
Frank Pospiech  
Geschäftsführer – Managing Director

## O2-Erklärung O2 Declaration

Wärmetauscher für den Einsatz mit  
hochreinem Sauerstoff optimiert

*Heat Exchanger optimised for use with  
high-purity oxygen*

**Applikationen mit Sauerstoff: Partikel-, Öl- und Fettfreiheit**

Mit dieser Erklärung bestätigen wir, dass alle medienberührenden Flächen der nachfolgenden Produkte in Anlehnung an die Vorgaben der EIGA Doc 33/18 und des VDA-Band 19 gereinigt und gefertigt sind.

***Applications with oxygen: free of particles, oil and grease***

*With this declaration, we confirm that all surfaces of the following products that come into contact with media have been cleaned and manufactured in accordance with the specifications of EIGA Doc 33/18 and VDA Volume 19.*

Produkt / Products	Wärmetauscher / Heat Exchanger	Art-Nr. / Item no.:
Typen / Types:	PTS-O2	4447999-O2
	PTS-I-O2	4448999I-O2
	TS-O2	4510023-O2
	TS-I-O2	4510025I-O2
	DTS-O2	4501026-O2
	DTS-I-O2	4501026I-O2

Ratingen, den 25.04.2024

Bühler Technologies GmbH





# Heat exchanger optimized for use with high-purity oxygen

## Applications with oxygen: Free from particles, oil and grease



For use with high-purity oxygen, the product requires special cleaning to ensure that it is free from oil and grease, as oxygen is a strong oxidising agent. Under unfavourable conditions, oxygen can cause spontaneous combustion of organic substances such as particles, oils and fats, and generally promotes the combustion of substances. Oils and fats can even react explosively on contact with oxygen. We use special cleaning and production processes to ensure the safe use of our products with high-purity oxygen and to avoid the above-mentioned undesirable reactions.

With this declaration, we confirm that all surfaces of the following products that come into contact with media have been cleaned and manufactured in accordance with the requirements of EIGA Doc 33/18 and VDA Volume 19.

Product:	Heat exchanger	Item no.
Models:	PTS-O2	4447999-O2
	PTS-I-O2	4448999I-O2
	TS-O2	4510023-O2
	TS-I-O2	4510025I-O2
	DTS-O2	4501026-O2
	DTS-I-O2	4501026I-O2

The material used for the “O2” heat exchangers is high-quality stainless steel, which has been tested by Bühler Technologies for its suitability for oxygen applications.

All components in contact with the medium undergo a special cleaning process to reliably remove impurities (such as oil, grease and particles). This process is documented by a comprehensive delivery specification to the service provider and compliance with the limits is verified with regular analyses by an independent, accredited laboratory.

The contamination limits of the surfaces in contact with media are defined as follows (as in EIGA Doc 33/18 Cleaning of Equipment for oxygen service):

	Contamination limits
Non-volatile organic or inorganic impurities:	$\leq 220 \text{ mg/m}^2$ for non-volatile impurities
Particles:	$\leq 22 \text{ particles/m}^2$ between $500 \mu\text{m}$ and $1000 \mu\text{m}$

The component groups of the heat exchangers are cleaned by an external service provider and then manufactured into the end product at Bühler Technologies. After these production steps, the heat exchanger undergoes final cleaning by the service provider before delivery in order to remove any contamination from the production process.

Compliance with the contamination limits is documented by the external service provider by means of factory test certificates (free of oil and grease) and a test report (free of dust and dirt). After cleaning, the heat exchangers are packed in airtight and dustproof packaging and clearly labeled “Cleaned for oxygen service. Do not open until ready for use”.

All described cleaning properties are lost if the product comes into contact with oily or greasy media or is otherwise contaminated from the outside.





# CERTIFICATE OF CONFORMITY



1. **HAZARDOUS LOCATION ELECTRICAL EQUIPMENT PER CANADIAN REQUIREMENTS**
2. **Certificate No:** FM18CA0010X
3. **Equipment:** TC-Standard X2; TC-Standard+ X2; TC-MIDI X2; TC MIDI+ X2; TC-Double X2 & TC-Double+ X2  
**(Type Reference and Name)** Sample Gas Cooler
4. **Name of Listing Company:** Bühler Technologies GmbH
5. **Address of Listing Company:** Harkortstrasse 29  
Ratingen, D-40880  
Germany
6. The examination and test results are recorded in confidential report number:  
  
3062014 dated 4<sup>th</sup> October 2018
7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:  
  
CSA-C22.2 No. 213-15, CAN/CSA-C22.2 No. 61010-1:2012
8. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.
9. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.
10. **Equipment Ratings:**  
  
**TC-Standard Models:**  
  
Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous locations with an ambient temperature rating of 0°C of up to 50°C.

## Certificate issued by:

J.E. Marquedant  
VP, Manager, Electrical Systems

4 October 2018

Date

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC, 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA  
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmapprovals.com](mailto:information@fmapprovals.com) [www.fmapprovals.com](http://www.fmapprovals.com)

# SCHEDULE



Canadian Certificate Of Conformity No: FM18CA0010X

## **TC-MIDI and TC-Double Models:**

Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous (classified) locations with an ambient temperature rating of 0°C of up to 60°C.

11. The marking of the equipment shall include:

## **TC-Standard Models:**

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

## **TC-MIDI and TC-Double Models:**

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

12. **Description of Equipment:**

**General** - The TC-6 sample gas chillers are intended to cool and dry the sample gas before going into the gas analysers. Sample gases contain vapour which has to be withdrawn before it reaches the gas analyser. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a preset temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

**Construction** – The equipment is housed in a brushed stainless steel IP20 enclosure.

**Ratings** - TC-Standard operate at 24VDC, 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 50°C. and TC-MIDI and TC-Double Models operate at 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 60°C.

## **4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)**

- b = Gas cooler model: 1 or 2
- d, = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 1, 3
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

## **4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)**

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 2, or 4
- j & k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, 22

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

# SCHEDULE



Canadian Certificate Of Conformity No: FM18CA0010X

- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

## **4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)**

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 22, 27, 32 & 37
- h = Peristaltic Pumps; 0, 2, 4
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = no value assigned.

## **4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI + X2(fitted with 1 heat exchangers)**

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- e = Gas paths; 1 or 2
- f,g = Heat exchangers; 60,61, 65, 66, 70, 75, 80 or 85
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20 21, or 22
- l,m = Status output; 00 or 10
- n,o = Delta T control; 00 or 10

## **4496 312 b2d1fghijklm00 Thermoelectric Cooler, TC-MIDI + X2(fitted with 2 heat exchangers)**

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- f,g = Heat exchangers; 22, 27, 32, or 37
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, or 11
- l,m = Status output; 00 or 10

## **4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double X2**

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 10,15, 20,25,30, or 35
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

## **4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double+ X2**

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 22, 27, 32, or 37
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

# **SCHEDULE**



Canadian Certificate Of Conformity No: FM18CA0010X

**13. Specific Conditions of Use:**

1. *When installed as Class I Division 2 equipment, the thermoelectric cooler shall be mounted within a tool-secured IP54 enclosure.*

**14. Test and Assessment Procedure and Conditions:**

This Certificate has been issued in accordance with FM Approvals Canadian Certification Scheme.

**15. Schedule Drawings**

A copy of the technical documentation has been kept by FM Approvals.

**16. Certificate History**

Details of the supplements to this certificate are described below:

Date	Description
4 <sup>th</sup> October 2018	Original Issue.

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA  
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)



# CERTIFICATE OF CONFORMITY

## 1. HAZARDOUS LOCATION ELECTRICAL EQUIPMENT PER CANADIAN REQUIREMENTS

2. Certificate No: FM18CA0010X
3. Equipment:  
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2; TC-MIDI+ X2; TC-Double X2 & TC-Double+ X2 Sample Gas cooler
4. Name of Listing Company: Bühler Technologies GmbH
5. Address of Listing Company: Harkortstraße 29, Ratingen D-40880, Germany
6. The examination and test results are recorded in confidential report number:  
3062014 dated 4<sup>th</sup> October 2018

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

CSA C22.2 No. 213:2021, CSA C22.2 No. 61010-1:2019

8. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.
9. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.
10. Equipment Ratings:

**TC-Standard**

Nonincendive for Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

**TC-Midi & TC Double**

Nonincendive for Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

Certificate issued by:



J.E. Marquedant  
VP, Manager - Electrical Systems

9 October 2024

Date

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC, One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 348 (Jul 24)



## **SCHEDULE**

Canadian Certificate of Conformity No: FM18CA0010X

### **11. The marking of the equipment shall include:**

#### **TC-Standard**

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

#### **TC-Midi & TC Double**

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

### **12. Description of Equipment:**

**General** - The TC- Standard; TC-MIDI & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly). Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-MIDI X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-MIDI+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

**Construction** – The equipment is housed in a brushed stainless-steel IP20 enclosure.

**Ratings** - TC-Standard operate at 24VDC, 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 50°C. and TC-MIDI and TC-Double Models operate at 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 60°C.

See Annex for Model Codes

### **13. Specific Conditions of Use:**

1. When installed as Class I Division 2 equipment, the thermoelectric cooler shall be mounted within a tool-secured IP54 enclosure which is capable of accepting one or more of the Class I Division 2 wiring methods per the Canadian Electric Code (CSA C22.1).

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 348 (Jul 24)



## SCHEDULE

Canadian Certificate of Conformity No: FM18CA0010X

### 14. Test and Assessment Procedure and Conditions:

This Certificate has been issued in accordance with FM Approvals Canadian Certification Scheme.

### 15. Schedule Drawings

A copy of the technical documentation has been kept by FM Approvals.

### 16. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
4th October 2018	Original Issue.
9 October 2024	<u>Supplement 1:</u> Report Reference: RR242035 dated 9 October 2024. Description of the Change(s): <ol style="list-style-type: none"><li>1. Addition of product variants due to changes to electronics</li><li>2. CSA C22.2 No. 213:2015 updated to CSA C22.2 No. 213:2021</li><li>3. CSA C22.2 No. 61010-1:2012 updated to CSA C22.2 No. 61010-1:2019</li></ol>

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 348 (Jul 24)



## SCHEDULE

Canadian Certificate of Conformity No: FM18CA0010X

**FM** Approvals

# ANNEX

## **4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)**

### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35  
h = Condensate drain; 00, 10 or 30  
j & k = Moisture detector/Filter; 00, 01, 10, or 11  
l = Status Outputs; 00 or 10  
n = Delta T control; 00 or 10

## **4496 211b2d1fg0000l0n0p TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchanger for H2/O2 applications)**

### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1 or 2  
f, g = Heat exchanger; 10, 15, 10 or 15  
l = Status Outputs; 00 or 10  
n = Delta T control; 00 or 10  
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

## **4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)**

### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35  
h = Condensate drain; 0, 2, or 4  
j & k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21, 22  
l = Status Outputs; 0 or 1  
n = Delta T control; 0 or 1

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 348 (Jul 24)





## SCHEDULE

Canadian Certificate of Conformity No: FM18CA0010X

**FM** Approvals

### **4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)**

#### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 22, 27, 32 or 37  
h = Condensate drain; 0, 2, 4  
j & k = Moisture detector/Filter; 00, 01, 10, or 11  
l = Signal Outputs; 0 or 1  
n = no value assigned.

### **4496 311 b2defghijklmno TC-MIDI X2(fitted with 1 heat exchangers)**

#### **Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
e = Gas path; 1 or 2  
f,g = Heat exchangers; 10, 15, 20, 25, 30 or 35  
h = Condensate drain; 0, 1 or 3  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector/Filter; 00, 01, 10 or 11  
l,m = Signal output; 00 or 10  
n,o = Delta T control; 00 or 10

### **4496 311 b2defg0000lmnop TC-MIDI X2 (fitted with 1 heat exchangers for H2/O2 applications)**

#### **Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
e = Gas path; 1 or 2  
f,g = Heat exchangers; 10, 15, 60, 65  
l,m = Signal output; 00 or 10  
n,o = Delta T control; 00 or 10  
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 348 (Jul 24)



## SCHEDULE

Canadian Certificate of Conformity No: FM18CA0010X

**FM Approvals**

### **4496 312 b2d1fghijklm00 TC-MIDI + X2(fitted with 2 heat exchangers)**

#### **Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
f,g = Heat exchangers; 60, 65, 61, 66, 70, 75, 80 or 85  
h = Condensate drain; 0, 2, or 4  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21 or 22  
l,m = Signal outputs; 00 or 10  
n, o = Delta T Control; 00 or 10

### **4496 611a2c1efghijkl000 TC-Double X2**

#### **Description of Equipment:**

a = Gas cooler types 1 or 2  
c = Voltage; 1 or 2  
e,f = Heat exchangers; 10, 15, 20, 25, 30 or 35  
g = Condensate drain; 0, 2, or 4  
h = Sample gas pumps; 0, 1, or 2  
i,j = Humidity sensor/Filter; 00, 01, 10, or 11  
k,l = Signal outputs; 00 or 10

### **4496 611a2c1efghijkl000 TC-Double+ X2**

#### **Description of Equipment:**

a = Gas cooler types 1 or 2  
c = Voltage; 1 or 2  
e,f = Heat exchangers; 22, 27, 32, or 37  
g = Peristaltic pumps; 0, 2, or 4  
h = Sample gas pumps; 0, 1, or 2  
i,j = Moisture Detector/Filter; 00, 01, 10, or 11  
k,l = Status output; 00 or 10

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 348 (Jul 24)




Page 6 of 6

# CERTIFICATE OF CONFORMITY



1. **HAZARDOUS (CLASSIFIED) LOCATION ELECTRICAL EQUIPMENT PER US REQUIREMENTS**
2. **Certificate No:** FM18US0021X
3. **Equipment:** C-Standard X2; TC-Standard+ X2; TC-MIDI X2; TC MIDI+ X2;  
**(Type Reference and Name)** TC-Double X2 & TC-Double+ X2  
Sample Gas cooler
4. **Name of Listing Company:** Bühler Technologies GmbH
5. **Address of Listing Company:** Harkortstrasse 29  
Ratingen, D-40880  
Germany
6. The examination and test results are recorded in confidential report number:  
  
3062014 dated 4<sup>th</sup> October 2018
7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:  
  
FM Class 3600:2018, FM Class 3611:2018, FM Class 3810:2018,  
ANSI/ISA-12.12.01-2015, ANSI/ISA 61010-1:2012
8. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.
9. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.
10. **Equipment Ratings:**  
  
**TC-Standard Models:**  
  
Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous (classified) locations with an ambient temperature rating of 0°C to 50°C.

## Certificate issued by:



J.E. Marquedant  
VP, Manager, Electrical Systems

4 October 2018

Date

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC, 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA  
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmapprovals.com](mailto:information@fmapprovals.com) [www.fmapprovals.com](http://www.fmapprovals.com)

# SCHEDULE



US Certificate Of Conformity No: FM18US0021X

## **TC-MIDI and TC-Double Models:**

Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous (classified) locations with an ambient temperature rating of 0°C to 60°C.

11. The marking of the equipment shall include:

## **TC-Standard Models:**

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

## **TC-MIDI and TC-Double Models:**

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

12. **Description of Equipment:**

**General** - The TC- Standard; TC-Midi & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-Midi X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-Midi+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

**Construction** – The equipment is housed in a brushed stainless IP20 enclosure.

**Ratings** - TC-Standard operate at 24VDC, 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C up to 50°C. and TC-MIDI and TC-Double Models operate at 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C up to 60°C.

**4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)**

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)



# SCHEDULE



US Certificate Of Conformity No: FM18US0021X

- b = Gas cooler model: 1 or 2
- d, = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 1, 3
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

## **4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)**

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 2, or 4
- j & k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, 22
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

## **4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)**

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 22, 27, 32 & 37
- h = Peristaltic Pumps; 0, 2, 4
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = no value assigned.

## **4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI + X2(fitted with 1 heat exchangers)**

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- e = Gas paths; 1 or 2
- f,g = Heat exchangers; 60, 61, 65, 66, 70, 75, 80 or 85
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, or 22
- l,m = Status output; 00 or 10
- n,o = Delta T control; 00 or 10

## **4496 312 b2d1fghijklm00 Thermoelectric Cooler, TC-MIDI + X2(fitted with 2 heat exchangers)**

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- f,g = Heat exchangers; 22, 27, 32, or 37
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, or 11
- l,m = Status output; 00 or 10

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

# **SCHEDULE**



US Certificate Of Conformity No: FM18US0021X

## **4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double X2**

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 10,15, 20,25,30, or 35
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

## **4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double+ X2**

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 22, 27, 32, or 37
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

### **13. Specific Conditions of Use:**

1. *When installed as Class I Division 2 equipment, the thermoelectric cooler shall be mounted within a tool-secured IP54 enclosure which is capable of accepting one or more of the Class I Division 2 wiring methods per the National Electric Code (ANSI/NFPA 70).*

### **14. Test and Assessment Procedure and Conditions:**

This Certificate has been issued in accordance with FM Approvals US Certification Requirements.

### **15. Schedule Drawings**

A copy of the technical documentation has been kept by FM Approvals.

### **16. Certificate History**

Details of the supplements to this certificate are described below:

Date	Description
4 <sup>th</sup> October 2018	Original Issue.

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA  
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

# CERTIFICATE OF CONFORMITY



1. **HAZARDOUS (CLASSIFIED) LOCATION ELECTRICAL EQUIPMENT PER US REQUIREMENTS**

2. **Certificate No:** FM18US0021X

3. **Equipment:** TC-Standard X2; TC-Standard+ X2; TC-MIDI X2; TC MIDI+ X2; TC-Double X2 & TC-Double+ X2

(Type Reference and Name)  
**Sample Gas cooler**  
4. **Name of Listing Company:** Bühler Technologies GmbH

5. **Address of Listing Company:** Harkortstrasse 29  
Ratingen, D-40880  
Germany

6. The examination and test results are recorded in confidential report number:

3062014 dated 4<sup>th</sup> October 2018

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

FM Class 3600:2018, FM Class 3611:2018, FM Class 3810:2018,  
ANSI/ISA-12.12.01-2015, ANSI/ISA 61010-1:2012

8. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

9. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.

10. Equipment Ratings:

**TC-Standard Models:**

Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous (classified) locations with an ambient temperature rating of 0°C to 50°C.

**Certificate issued by:**

J.E. Marquedant  
VP, Manager - Electrical Systems

25 January 2021

Date

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC, 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA  
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmapprovals.com](mailto:information@fmapprovals.com) [www.fmapprovals.com](http://www.fmapprovals.com)

# SCHEDULE



US Certificate Of Conformity No: FM18US0021X

## **TC-MIDI and TC-Double Models:**

Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous (classified) locations with an ambient temperature rating of 0°C to 60°C.

11. The marking of the equipment shall include:

## **TC-Standard Models:**

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

## **TC-MIDI and TC-Double Models:**

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

12. **Description of Equipment:**

**General** - The TC- Standard; TC-Midi & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-Midi X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-Midi+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

**Construction** – The equipment is housed in a brushed stainless IP20 enclosure.

**Ratings** - TC-Standard operate at 24VDC, 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 50°C. and TC-MIDI and TC-Double Models operate at 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 60°C.

**4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)**

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)



# SCHEDULE



US Certificate Of Conformity No: FM18US0021X

- b = Gas cooler model: 1 or 2
- d, = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 1, 3
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

**4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)**

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 2, or 4
- j & k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, 22
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

**4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)**

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 22, 27, 32 & 37
- h = Peristaltic Pumps; 0, 2, 4
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = no value assigned.

**4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI X2(fitted with 1 heat exchangers)**

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- e = Gas paths; 1 or 2
- f,g = Heat exchangers; 60, 61, 65, 66, 70, 75, 80 or 85
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, or 22
- l,m = Status output; 00 or 10
- n,o = Delta T control; 00 or 10

**4496 312 b2d1fghijklm00 Thermoelectric Cooler, TC-MIDI + X2(fitted with 2 heat exchangers)**

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- f,g = Heat exchangers; 22, 27, 32, or 37
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, or 11
- l,m = Status output; 00 or 10

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

# SCHEDULE



US Certificate Of Conformity No: FM18US0021X

**4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double X2**

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 10, 15, 20, 25, 30, or 35
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

**4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double+ X2**

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 22, 27, 32, or 37
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

**13. Specific Conditions of Use:**

1. *When installed as Class I Division 2 equipment, the thermoelectric cooler shall be mounted within a tool-secured IP54 enclosure which is capable of accepting one or more of the Class I Division 2 wiring methods per the National Electric Code (ANSI/NFPA 70).*

**14. Test and Assessment Procedure and Conditions:**

This Certificate has been issued in accordance with FM Approvals US Certification Requirements.

**15. Schedule Drawings**

A copy of the technical documentation has been kept by FM Approvals.

**16. Certificate History**

Details of the supplements to this certificate are described below:

Date	Description
4 <sup>th</sup> October 2018	Original Issue.
25 <sup>th</sup> January 2021	Supplement 1: Report Reference: RR226270 dated 25 <sup>th</sup> January 2021. Description of the Change: Add digital interface and correct typo in model code to remove + for TC-MIDI fitted with 1 heat exchanger.

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA  
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

# **SCHEDULE**



US Certificate Of Conformity No: FM18US0021X

FM Approvals

FM Approvals

FM Approvals

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA  
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

# CERTIFICATE OF CONFORMITY

## 1. HAZARDOUS (CLASSIFIED) LOCATION ELECTRICAL EQUIPMENT PER US REQUIREMENTS

2. Certificate No: FM18US0021X
3. Equipment:  
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2; TC-MIDI+ X2; TC-Double X2 & TC-Double+ X2  
Sample Gas cooler
4. Name of Listing Company: Bühler Technologies GmbH
5. Address of Listing Company: Harkortstraße 29, Ratingen D-40880, Germany
6. The examination and test results are recorded in confidential report number:

3062014 dated 4<sup>th</sup> October 2018

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

FM 3600:2022, FM 3611:2021, FM 3810:2021, ANSI/UL 61010-1:2019, ANSI/UL 121201:2021

8. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.
9. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.
10. Equipment Ratings:

**TC-Standard**

Nonincendive for Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

**TC-Midi & TC Double**

Nonincendive for Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

Certificate issued by:



J.E. Marquedant  
VP, Manager - Electrical Systems

9 October 2024

Date

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC, One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 347 (Jul 24)





## **SCHEDULE**

US Certificate of Conformity No: FM18US0021X

### **11. The marking of the equipment shall include:**

#### **TC-Standard**

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

#### **TC-Midi & TC Double**

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

### **12. Description of Equipment:**

**General** - The TC- Standard; TC-MIDI & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly). Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-MIDI X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-MIDI+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

**Construction** – The equipment is housed in a brushed stainless-steel IP20 enclosure.

**Ratings** - TC-Standard operate at 24VDC, 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 50°C. and TC-MIDI and TC-Double Models operate at 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 60°C.

See Annex for Model Codes

### **13. Specific Conditions of Use:**

1. When installed as Class I Division 2 equipment, the thermoelectric cooler shall be mounted within a tool-secured IP54 enclosure which is capable of accepting one or more of the Class I Division 2 wiring methods per the National Electric Code (ANSI/NFPA 70).

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 347 (Jul 24)



## **SCHEDULE**

US Certificate of Conformity No: FM18US0021X

### **14. Test and Assessment Procedure and Conditions:**

This Certificate has been issued in accordance with FM Approvals US Certification Requirements.

### **15. Schedule Drawings**

A copy of the technical documentation has been kept by FM Approvals.

### **16. Certificate History**

Details of the supplements to this certificate are described below:

Date	Description
4 October 2018	Original Issue.
25 January 2021	<u>Supplement 1:</u> Report Reference: RR226270 dated 25 <sup>th</sup> January 2021. Description of the Change: Add digital interface and correct typo in model code to remove + for TC-MIDI fitted with 1 heat exchanger.
9 October 2024	<u>Supplement 2:</u> Report Reference: RR242035 dated 9 October 2024. Description of the Change(s): <ol style="list-style-type: none"><li>1. Addition of product variants due to changes to electronics</li><li>2. FM3600 updated to latest edition (2022)</li><li>3. FM3611 updated to latest edition (2021)</li><li>4. FM3810 updated to latest edition (2021)</li><li>5. ANSI/UL 121201:2015 updated to ANSI/UL 121201:2021</li><li>6. ANSI/ISA 61010-1:2012 updated to ANSI/UL 61010-1:2019</li></ol>

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 347 (Jul 24)



## **SCHEDULE**

US Certificate of Conformity No: FM18US0021X

**FM Approvals**

# **ANNEX**

## **4496 211b2d11gh0jkl0n0pTC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchanger)**

### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35  
h = Condensate drain; 00, 10 or 30  
j & k = Moisture detector/Filter; 00, 01, 10, or 11  
l = Status Outputs; 00 or 10  
n = Delta T control; 00 or 10

## **4496 211b2d1fg0000l0n0p TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchanger for H2/O2 applications)**

### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1 or 2  
f, g = Heat exchanger; 10, 15, 10 or 15  
l = Status Outputs; 00 or 10  
n = Delta T control; 00 or 10  
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

## **4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)**

### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35  
h = Condensate drain; 0, 2, or 4  
j & k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21, 22  
l = Status Outputs; 0 or 1  
n = Delta T control; 0 or 1

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 347 (Jul 24)



## **SCHEDULE**

US Certificate of Conformity No: FM18US0021X

**FM Approvals**

### **4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)**

#### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 22, 27, 32 or 37  
h = Condensate drain; 0, 2, 4  
j & k = Moisture detector/Filter; 00, 01, 10, or 11  
l = Signal Outputs; 0 or 1  
n = no value assigned.

### **4496 311 b2defghijklmno TC-MIDI X2(fitted with 1 heat exchangers)**

#### **Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
e = Gas path; 1 or 2  
f,g = Heat exchangers; 10, 15, 20, 25, 30 or 35  
h = Condensate drain; 0, 1 or 3  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector/Filter; 00, 01, 10 or 11  
l,m = Signal output; 00 or 10  
n,o = Delta T control; 00 or 10

### **4496 311 b2defg0000lmnop TC-MIDI X2 (fitted with 1 heat exchangers for H2/O2 applications)**

#### **Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
e = Gas path; 1 or 2  
f,g = Heat exchangers; 10, 15, 60, 65  
l,m = Signal output; 00 or 10  
n,o = Delta T control; 00 or 10  
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 347 (Jul 24)





## **SCHEDULE**

US Certificate of Conformity No: FM18US0021X

**FM Approvals**

### **4496 312 b2d1fghijklm00 TC-MIDI + X2(fitted with 2 heat exchangers)**

#### **Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
f,g = Heat exchangers; 60, 65, 61, 66, 70, 75, 80 or 85  
h = Condensate drain; 0, 2, or 4  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21 or 22  
l,m = Signal outputs; 00 or 10  
n, o = Delta T Control; 00 or 10

### **4496 611a2c1efghijkl000 TC-Double X2**

#### **Description of Equipment:**

a = Gas cooler types 1 or 2  
c = Voltage; 1 or 2  
e,f = Heat exchangers; 10, 15, 20, 25, 30 or 35  
g = Condensate drain; 0, 2, or 4  
h = Sample gas pumps; 0, 1, or 2  
i,j = Humidity sensor/Filter; 00, 01, 10, or 11  
k,l = Signal outputs; 00 or 10

### **4496 611a2c1efghijkl000 TC-Double+ X2**

#### **Description of Equipment:**

a = Gas cooler types 1 or 2  
c = Voltage; 1 or 2  
e,f = Heat exchangers; 22, 27, 32, or 37  
g = Peristaltic pumps; 0, 2, or 4  
h = Sample gas pumps; 0, 1, or 2  
i,j = Moisture Detector/Filter; 00, 01, 10, or 11  
k,l = Status output; 00 or 10

To verify the availability of the Approved product, please refer to [www.approvalguide.com](http://www.approvalguide.com)

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: [information@fmaprovals.com](mailto:information@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F 347 (Jul 24)



# 1 TYPE EXAMINATION CERTIFICATE



2 Equipment or Protective systems intended for use in Potentially  
Explosive Atmospheres - Directive 2014/34/EU

3 Type Examination Certificate No: FM18ATEX0012X

4 Equipment or protective system:  
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2;  
TC MIDI+ X2; TC-Double X2 & TC-Double+ X2  
Sample Gas Cooler

5 Name of Applicant: Bühler Technologies GmbH

6 Address of Applicant: Harkortstrasse 29  
Ratingen, D-40880  
Germany

7 This equipment or protective system and any acceptable variation thereto is specified in the schedule to this certificate and documents therein referred to.

8 FM Approvals Europe Ltd. certifies that this equipment has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment intended for use in potentially explosive atmospheres given in Annex II to the Directive.

The examination and test results are recorded in confidential report number:

3062014 dated 04<sup>th</sup> October 2018

9 Compliance with the Essential Health and Safety Requirements, with the exception of those identified in item 15 of the schedule to this certificate, has been assessed by compliance with the following documents:

EN 60079-0:2012+A11:2013, EN 60079-7:2015+A1:2018 & EN 60079-15:2018

10 If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

11 This Type Examination certificate relates only to the design, examination and tests of the specified equipment or protective system in accordance to the Directive 2014/34/EU. Further requirements of the Directive apply to the manufacturing process and supply of this equipment or protective system. These are not covered by this certificate.

12 The marking of the equipment or protective system shall include:



II 3 G Ex ec nC IIC T4 Gc

Ta = 0°C to +40°C or 0°C to +50°C (TC-Standard X2 & TC-Standard+ X2 Models)

Ta = 0°C to +40°C or 0°C to +60°C (TC-MIDI X2 & TC-MIDI+ X2 and  
TC-Double X2 & TC-Double+ X2 Models)

  
FM Approvals  
Member of the FM Global Group

Digitally signed by Damien Mc Ardle  
DN: cn=Damien Mc Ardle, o=FM  
Approvals, ou=FM Approvals Europe  
Ltd,  
email=damien.mcardle@fmapproval  
s.com, c=IE  
Date: 2020.02.18 18:14:19 Z

**Damien Mc Ardle**  
Certification Manager, FM Approvals Europe Ltd.

Issue date: 18<sup>th</sup> February 2020

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440  
T: +353 (0) 1761 4200 E-mail: [atex@fmapprovals.com](mailto:atex@fmapprovals.com) [www.fmapprovals.com](http://www.fmapprovals.com)

# SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

## 13 Description of Equipment or Protective System:

The TC- Standard; TC-Midi & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analysers. Sample gases contain vapour which has to be withdrawn before it reaches the gas analyser. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-Midi X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-Midi+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimise wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimise wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

### **TC-Standard X2 - Sample Gas Cooler (fitted with 1 or 2 heat exchangers)**

<b>Electrical data:</b> Umax 24VDC, 115VAC or 230 VAC, 50/60 Hz, TC – Standard Models	130 W
TC – MIDI Models	290 W
TC – Double models	390 W

### **4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)**

b	= Gas cooler model: 1 or 2
d,	= Supply voltage; 1, 2 or 4
f,g	= Heat exchanger; 10, 15, 20, 25, 30, or 35
h	= Peristaltic Pumps; 0, 1, 3
j,k	= Moisture detector / Filter; 00, 01, 10, or 11
l	= Status Outputs; 0 or 1
n	= Delta T control; 0 or 1

### **4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)**

b	= Gas cooler model: 1 or 2
d	= Supply voltage; 1, 2 or 4
f,g	= Heat exchanger; 10, 15, 20, 25, 30, or 35
h	= Peristaltic Pumps; 0, 2, or 4
j,k	= Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, 22
l	= Status Outputs; 0 or 1
n	= Delta T control; 0 or 1

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

# SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

**4496 212b2d2fgh0jkl000 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f,g = Heat exchanger; 22, 27, 32 or 37  
h = Peristaltic Pumps; 0, 2, 4  
j,k = Moisture detector / Filter; 00, 01, 10, or 11  
l = Status Outputs; 0 or 1

**4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI X2 (fitted with 1 gas path inside the heat exchanger)**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
e = Gas paths; 1 or 2  
f,g = Heat exchangers; 10, 15, 20, 25, 30, or 35  
h = Peristaltic pumps; 0, 1, or 3  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector / Filter; 00, 01, 10, or 11  
l,m = Status output; 00 or 10  
n,o = Delta T control; 00 or 10

**4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI X2 (fitted with 2 gas paths inside the heat exchanger)**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
e = Gas paths; 1 or 2  
f,g = Heat exchangers; 60, 61, 65, 66, 70, 75, 80 or 85  
h = Peristaltic pumps; 0, 2, or 4  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, or 22  
l,m = Status output; 00 or 10  
n,o = Delta T control; 00 or 10

**4496 312 b2d1fghijklmno Thermoelectric Cooler, TC-MIDI X2 (fitted with 2 heat exchangers)**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
f,g = Heat exchangers; 22, 27, 32, or 37  
h = Peristaltic pumps; 0, 2, or 4  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector / Filter; 00, 01, 10, or 11  
l,m = Status output; 00 or 10  
n,o = Delta T control; 00 or 10

**4496 312 b2d1fghijklm00 Thermoelectric Cooler, TC-MIDI + X2 (fitted with 2 heat exchangers in series)**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
f,g = Heat exchangers; 22, 27, 32, or 37  
h = Peristaltic pumps; 0, 2, or 4  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector / Filter; 00, 01, 10, or 11  
l,m = Status output; 00 or 10

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**



# SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

**4496 611a2c1efghijk000 Thermoelectric Cooler, TC-Double X2 (fitted with 2 heat exchangers in series)**

- a = Gas cooler types 1, 2, 3 or 4
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 10,15, 20,25,30, or 35
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k = Status output; 0 or 1

**4496 611a2c1efghijk000 Thermoelectric Cooler, TC-Double+ X2**

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 22, 27, 32, or 37
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11

**14 Specific Conditions of Use:**

1. *The equipment shall be mounted in an enclosure providing a minimum degree of protection of IP54 in accordance with EN 60079-15, and in a tool-secured enclosure which meets the requirements of EN 60079-0 and EN 60079-15.*

**15 Essential Health and Safety Requirements:**

The relevant EHSRs that have not been addressed by the standards listed in this certificate have been identified and assessed in the confidential report identified in item 8.

**16 Test and Assessment Procedure and Conditions:**

This Type Examination Certificate is the result of testing of a sample of the product submitted, in accordance with the provisions of the relevant specific standard(s), and assessment of supporting documentation. It does not imply an assessment of the whole production.

Whilst this certificate may be used in support of a manufacturer's claim for CE Marking, FM Approvals Europe Ltd accepts no responsibility for the compliance of the equipment against all applicable Directives in all applications.

This Certificate has been issued in accordance with FM Approvals Europe Ltd's ATEX Certification Scheme.

**17 Schedule Drawings**

A list of the significant parts of the technical documentation is annexed to this certificate and a copy has been kept by FM Approvals Europe Ltd.

**18 Certificate History**

Details of the supplements to this certificate are described below:

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

# **SCHEDULE**

to Type Examination Certificate No. FM18ATEX0012X

Date	Description
15 <sup>th</sup> October 2018	Original Issue.
18 <sup>th</sup> February 2020	<u>Supplement 1:</u> Report Reference: RR222218 dated 17 <sup>th</sup> February 2020. Description of the Change: <ol style="list-style-type: none"><li>1. A correction of typographical errors in model code section and the electrical power ratings.</li><li>2. Certificate transferred from FM Approvals Ltd., notified body no. 1725, to FM Approvals Europe Ltd., notified body no. 2809</li><li>3. Update CDL</li></ol>

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440  
T: +353 (0) 1761 4200 E-mail: [atex@fmaprovals.com](mailto:atex@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)



# 1 TYPE EXAMINATION CERTIFICATE

2 Equipment or Protective systems intended for use in Potentially  
Explosive Atmospheres - Directive 2014/34/EU

3 Type Examination Certificate No: FM18ATEX0012X

4 Equipment or protective system:  
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2;  
TC MIDI+ X2; TC-Double X2 & TC-Double+ X2  
Sample Gas Cooler

5 Name of Applicant: Bühler Technologies GmbH

6 Address of Applicant: Harkortstrasse 29  
Ratingen, D-40880  
Germany

7 This equipment or protective system and any acceptable variation thereto is specified in the schedule to this certificate and documents therein referred to.

8 FM Approvals Europe Ltd. certifies that this equipment has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment intended for use in potentially explosive atmospheres given in Annex II to the Directive.

The examination and test results are recorded in confidential report number:

3062014 dated 04<sup>th</sup> October 2018

9 Compliance with the Essential Health and Safety Requirements, with the exception of those identified in item 15 of the schedule to this certificate, has been assessed by compliance with the following documents:

EN 60079-0:2012+A11:2013, EN 60079-7:2015+A1:2018 and EN 60079-15:2018

10 If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

11 This Type Examination certificate relates only to the design, examination and tests of the specified equipment or protective system in accordance to the Directive 2014/34/EU. Further requirements of the Directive apply to the manufacturing process and supply of this equipment or protective system. These are not covered by this certificate.

12 The marking of the equipment or protective system shall include:



II 3 G Ex ec nC IIC T4 Gc

Ta = 0°C to +40°C or 0°C to +50°C (TC-Standard X2 & TC-Standard+ X2 Models)

Ta = 0°C to +40°C or 0°C to +60°C (TC-MIDI X2 & TC-MIDI+ X2 and  
TC-Double X2 & TC-Double+ X2 Models)

*Damien McArdle*

**Damien Mc Ardle**  
Certification Manager, FM Approvals Europe Ltd.

Issue date: 26<sup>th</sup> January 2021

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**



FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440  
T: +353 (0) 1761 4200 E-mail: [atex@fmaprovals.com](mailto:atex@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)

F ATEX 029 (Mar/2019)

Page 1 of 5

# SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

## 13 Description of Equipment or Protective System:

The TC- Standard; TC-Midi & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analysers. Sample gases contain vapour which has to be withdrawn before it reaches the gas analyser. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-Midi X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-Midi+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimise wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimise wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set to different temperatures.

### **TC-Standard X2 - Sample Gas Cooler (fitted with 1 or 2 heat exchangers)**

<b>Electrical data:</b> Umax 24VDC, 115VAC or 230 VAC, 50/60 Hz, TC – Standard Models	130 W
TC – MIDI Models	290 W
TC – Double models	390 W

### **4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)**

- b = Gas cooler model: 1 or 2
- d, = Supply voltage; 1, 2 or 4
- f,g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 1, 3
- j,k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

### **4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)**

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f,g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 2, or 4
- j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, 22
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**



# SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

**4496 212b2d2fgh0jkl000 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)**

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f,g = Heat exchanger; 22, 27, 32 or 37
- h = Peristaltic Pumps; 0, 2, 4
- j,k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1

**4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI X2 (fitted with 1 gas path inside the heat exchanger)**

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- e = Gas paths; 1 or 2
- f,g = Heat exchangers; 10, 15, 20, 25, 30, or 35
- h = Peristaltic pumps; 0, 1, or 3
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 10, or 11
- l,m = Status output; 00 or 10
- n,o = Delta T control; 00 or 10

**4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI + X2 (fitted with 2 gas paths inside the heat exchanger)**

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- e = Gas paths; 1 or 2
- f,g = Heat exchangers; 60, 61, 65, 66, 70, 75, 80 or 85
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, or 22
- l,m = Status output; 00 or 10
- n,o = Delta T control; 00 or 10

**4496 312 b2d1fghijklmno Thermoelectric Cooler, TC-MIDI X2 (fitted with 2 heat exchangers)**

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- f,g = Heat exchangers; 22, 27, 32, or 37
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 10, or 11
- l,m = Status output; 00 or 10
- n,o = Delta T control; 00 or 10

**4496 312 b2d1fghijklm00 Thermoelectric Cooler, TC-MIDI + X2 (fitted with 2 heat exchangers in series)**

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- f,g = Heat exchangers; 22, 27, 32, or 37
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 10, or 11
- l,m = Status output; 00 or 10

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

# SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

**4496 611a2c1efghijk000 Thermoelectric Cooler, TC-Double X2 (fitted with 2 heat exchangers in series)**

- a = Gas cooler types 1, 2, 3 or 4
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 10, 15, 20, 25, 30, or 35
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k = Status output; 0 or 1

**4496 611a2c1efghijk000 Thermoelectric Cooler, TC-Double+ X2**

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 22, 27, 32, or 37
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11

**14 Specific Conditions of Use:**

1. *The equipment shall be mounted in an enclosure providing a minimum degree of protection of IP54 in accordance with EN 60079-15, and in a tool-secured enclosure which meets the requirements of EN 60079-0 and EN 60079-15.*

**15 Essential Health and Safety Requirements:**

The relevant EHSRs that have not been addressed by the standards listed in this certificate have been identified and assessed in the confidential report identified in item 8.

**16 Test and Assessment Procedure and Conditions:**

This Type Examination Certificate is the result of testing of a sample of the product submitted, in accordance with the provisions of the relevant specific standard(s), and assessment of supporting documentation. It does not imply an assessment of the whole production.

Whilst this certificate may be used in support of a manufacturer's claim for CE Marking, FM Approvals Europe Ltd accepts no responsibility for the compliance of the equipment against all applicable Directives in all applications.

This Certificate has been issued in accordance with FM Approvals Europe Ltd's ATEX Certification Scheme.

**17 Schedule Drawings**

A list of the significant parts of the technical documentation is annexed to this certificate and a copy has been kept by FM Approvals Europe Ltd.

**18 Certificate History**

Details of the supplements to this certificate are described below:

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

# **SCHEDULE**

to Type Examination Certificate No. FM18ATEX0012X

Date	Description
15 <sup>th</sup> October 2018	Original Issue.
18 <sup>th</sup> February 2020	<u>Supplement 1:</u> Report Reference: RR222218 dated 17 <sup>th</sup> February 2020. Description of the Change: <ol style="list-style-type: none"><li>1. A correction of typographical errors in model code section and the electrical power ratings.</li><li>2. Certificate transferred from FM Approvals Ltd., notified body no. 1725, to FM Approvals Europe Ltd., notified body no. 2809</li><li>3. Update CDL</li></ol>
26 <sup>th</sup> January 2021	<u>Supplement 2:</u> Report Reference: RR226270 dated 25 <sup>th</sup> January 2021. Description of the Change: Add digital interface and correct typo in model code to remove + for TC-MIDI fitted with 1 heat exchanger.

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440  
T: +353 (0) 1761 4200 E-mail: [atex@fmaprovals.com](mailto:atex@fmaprovals.com) [www.fmaprovals.com](http://www.fmaprovals.com)



# 1. TYPE EXAMINATION CERTIFICATE

2. Equipment or Protective systems intended for use in Potentially Explosive Atmospheres - Directive 2014/34/EU

3. Type Examination Certificate No: FM18ATEX0012X

4. Equipment or protective system:  
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2;  
TC-MIDI+ X2; TC-Double X2 & TC-Double+ X2  
Sample Gas Cooler

5. Name of Applicant: Bühler Technologies GmbH

6. Address of Applicant Harkortstraße 29, Ratingen D-40880, Germany

7. This equipment or protective system and any acceptable variation thereto is specified in the schedule to this certificate and documents therein referred to.

8. FM Approvals Europe Ltd, certifies that this component has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment intended for use in potentially explosive atmospheres given in Annex II to the Directive.

The examination and test results are recorded in confidential report number:

3062014 dated 4<sup>th</sup> October 2018

9. Compliance with the Essential Health and Safety Requirements, with the exception of those identified in item 15 of the schedule to this certificate, has been assessed by compliance with the following documents:

EN IEC 60079-0:2018, EN 60079-7:2015+A1:2018, EN IEC 60079-15:2019

10. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

11. This Type Examination certificate relates only to the design, examination and tests of the specified equipment or protective system in accordance to the Directive 2014/34/EU. Further requirements of the Directive apply to the manufacturing process and supply of this equipment or protective system. These are not covered by this certificate.

Certificate issued by:

Certification Manager, FM Approvals Europe Ltd.

Date 10 October 2024

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440

T: +353 (0) 1761 4200 E-mail: [atex@fmapprovals.com](mailto:atex@fmapprovals.com) [www.fmapprovals.com](http://www.fmapprovals.com)

F ATEX 029 (Jul/2024)



Page 1 of 6



## **SCHEDULE**

to Type Examination Certificate No. FM18ATEX0012X

12. The marking of the equipment or protective system shall include:



**TC-Standard**

II 3 G Ex ec nC IIC T4 Gc

Ta = 0°C to +40°C or 0°C to +50°C

**TC-MIDI & TC Double**

II 3 G Ex ec nC IIC T4 Gc

Ta = 0°C to +40°C or 0°C to +60°C

13. **Description of Equipment or Protective System:**

The TC- Standard; TC-MIDI & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-MIDI X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-MIDI+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

TC-Standard X2 - Sample Gas Cooler (fitted with 1 or 2 heat exchangers)

**Electrical data:** Umax 24VDC, 115VAC or 230 VAC, 50/60 Hz

TC – Standard Models 130 W

TC – MIDI Models 290 W

TC – Double models 390 W

See Annex for Model Codes

14. **Specific Conditions of Use:**

1. The equipment shall be installed within a tool-secured enclosure providing a minimum degree of protection of IP54 and meeting the requirements of EN 60079-0 or certified as Ex e and in

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440

T: +353 (0) 1761 4200 E-mail: [atex@fmapprovals.com](mailto:atex@fmapprovals.com) [www.fmapprovals.com](http://www.fmapprovals.com)

F ATEX 029 (Jul/2024)

## **SCHEDULE**

to Type Examination Certificate No. FM18ATEX0012X

compliance with the enclosure, mounting, spacing and segregation requirements of the ultimate application.

### **15. Essential Health and Safety Requirements:**

The relevant EHSRs that have not been addressed by the standards listed in this certificate have been identified and assessed in the confidential report identified in item 8.

### **16. Test and Assessment Procedure and Conditions:**

This Type Examination Certificate is the result of testing of a sample of the product submitted, in accordance with the provisions of the relevant specific standard(s), and assessment of supporting documentation. It does not imply an assessment of the whole production.

Whilst this certificate may be used in support of a manufacturer's claim for CE Marking, FM Approvals Europe Ltd accepts no responsibility for the compliance of the equipment against all applicable Directives in all applications.

This Certificate has been issued in accordance with FM Approvals Europe Ltd's ATEX Certification Scheme.

### **17. Schedule Drawings**

A list of the significant parts of the technical documentation is annexed to this certificate and a copy has been kept by FM Approvals Europe Ltd.

### **18. Certificate History**

Details of the supplements to this certificate are described below:

Date	Description
15 October 2018	Original Issue.
18 February 2020	<u>Supplement 1:</u> Report Reference: RR222218 dated 17 <sup>th</sup> February 2020. Description of the Change: <ol style="list-style-type: none"><li>1. A correction of typographical errors in model code section and the electrical power ratings.</li><li>2. Certificate transferred from FM Approvals Ltd., notified body no. 1725, to FM Approvals Europe Ltd., notified body no. 2809</li><li>3. Update CDL</li></ol>
26 January 2021	<u>Supplement 2:</u> Report Reference: RR226270 dated 25 <sup>th</sup> January 2021. Description of the Change: Add digital interface and correct typo in model code to remove + for TC-MIDI fitted with 1 heat exchanger.
10 October 2024	<u>Supplement 3:</u> Report Reference: RR242035 dated 9 October 2024. Description of the Change(s): <ol style="list-style-type: none"><li>1. Addition of product variants due to changes to electronics</li><li>2. EN 60079-0:2012+A11:2013 updated to EN IEC 60079-0:2018</li></ol>

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

## **ANNEX**

### **4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)**

#### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35  
h = Condensate drain; 00, 10 or 30  
j & k = Moisture detector/Filter; 00, 01, 10, or 11  
l = Status Outputs; 00 or 10  
n = Delta T control; 00 or 10

### **4496 211b2d1fg0000l0n0p TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchanger for H<sub>2</sub>/O<sub>2</sub> applications)**

#### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1 or 2  
f, g = Heat exchanger; 10, 15, 10 or 15  
l = Status Outputs; 00 or 10  
n = Delta T control; 00 or 10  
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H<sub>2</sub> or -O<sub>2</sub>

### **4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)**

#### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35  
h = Condensate drain; 0, 2, or 4  
j & k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21, 22  
l = Status Outputs; 0 or 1  
n = Delta T control; 0 or 1

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

**4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)**

**Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 22, 27, 32 or 37  
h = Condensate drain; 0, 2, 4  
j & k = Moisture detector/Filter; 00, 01, 10, or 11  
l = Signal Outputs; 0 or 1  
n = no value assigned.

**4496 311 b2defghijklmno TC-MIDI X2(fitted with 1 heat exchangers)**

**Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
e = Gas path; 1 or 2  
f,g = Heat exchangers; 10, 15, 20, 25, 30 or 35  
h = Condensate drain; 0, 1 or 3  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector/Filter; 00, 01, 10 or 11  
l,m = Signal output; 00 or 10  
n,o = Delta T control; 00 or 10

**4496 311 b2defg0000lmnop TC-MIDI X2 (fitted with 1 heat exchangers for H2/O2 applications)**

**Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
e = Gas path; 1 or 2  
f,g = Heat exchangers; 10, 15, 60, 65  
l,m = Signal output; 00 or 10  
n,o = Delta T control; 00 or 10  
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**



## **4496 312 b2d1fghijklm00 TC-MIDI + X2(fitted with 2 heat exchangers)**

### **Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
f,g = Heat exchangers; 60, 65, 61, 66, 70, 75, 80 or 85  
h = Condensate drain; 0, 2, or 4  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21 or 22  
l,m = Signal outputs; 00 or 10  
n, o = Delta T Control; 00 or 10

---

## **4496 611a2c1efghijkl000 TC-Double X2**

### **Description of Equipment:**

a = Gas cooler types 1 or 2  
c = Voltage; 1 or 2  
e,f = Heat exchangers; 10, 15, 20, 25, 30 or 35  
g = Condensate drain; 0, 2, or 4  
h = Sample gas pumps; 0, 1, or 2  
i,j = Humidity sensor/Filter; 00, 01, 10, or 11  
k,l = Signal outputs; 00 or 10

---

## **4496 611a2c1efghijkl000 TC-Double+ X2**

### **Description of Equipment:**

a = Gas cooler types 1 or 2  
c = Voltage; 1 or 2  
e,f = Heat exchangers; 22, 27, 32, or 37  
g = Peristaltic pumps; 0, 2, or 4  
h = Sample gas pumps; 0, 1, or 2  
i,j = Moisture Detector/Filter; 00, 01, 10, or 11  
k,l = Status output; 00 or 10

---

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**



# 1. TYPE EXAMINATION CERTIFICATE

2. Equipment or Protective systems intended for use in Potentially Explosive Atmospheres - Directive 2014/34/EU

3. Type Examination Certificate No: FM18ATEX0012X

4. Equipment or protective system:  
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2;  
TC-MIDI+ X2; TC-Double X2 & TC-Double+ X2  
Sample Gas Cooler

5. Name of Applicant: Bühler Technologies GmbH

6. Address of Applicant Harkortstraße 29, Ratingen D-40880, Germany

7. This equipment or protective system and any acceptable variation thereto is specified in the schedule to this certificate and documents therein referred to.

8. FM Approvals Europe Ltd, certifies that this component has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment intended for use in potentially explosive atmospheres given in Annex II to the Directive.

The examination and test results are recorded in confidential report number:

3062014 dated 4<sup>th</sup> October 2018

9. Compliance with the Essential Health and Safety Requirements, with the exception of those identified in item 15 of the schedule to this certificate, has been assessed by compliance with the following documents:

EN IEC 60079-0:2018, EN 60079-7:2015+A1:2018, EN IEC 60079-15:2019

10. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

11. This Type Examination certificate relates only to the design, examination and tests of the specified equipment or protective system in accordance to the Directive 2014/34/EU. Further requirements of the Directive apply to the manufacturing process and supply of this equipment or protective system. These are not covered by this certificate.

Certificate issued by:

**FM Approvals**

6 December 2024

Certification Manager, FM Approvals Europe Ltd.

Date

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440  
T: +353 (0) 1761 4200 E-mail: [atex@fmapprovals.com](mailto:atex@fmapprovals.com) [www.fmapprovals.com](http://www.fmapprovals.com)  
F ATEX 029 (Jul/2024)



12. The marking of the equipment or protective system shall include:



**TC-Standard**

II 3 G Ex ec nC IIC T4 Gc  
Ta = 0°C to +40°C or 0°C to +50°C

**TC-MIDI & TC Double**

II 3 G Ex ec nC IIC T4 Gc  
Ta = 0°C to +40°C or 0°C to +60°C

**13. Description of Equipment or Protective System:**

The TC- Standard; TC-MIDI & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-MIDI X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-MIDI+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

TC-Standard X2 - Sample Gas Cooler (fitted with 1 or 2 heat exchangers)

**Electrical data:** Umax 24VDC, 115VAC or 230 VAC, 50/60 Hz

TC – Standard Models 130 W

TC – MIDI Models 290 W

TC – Double models 390 W

See Annex for Model Codes

**14. Specific Conditions of Use:**

1. The equipment shall be installed within a tool-secured enclosure providing a minimum degree of protection of IP54 and meeting the requirements of EN 60079-0 or certified as Ex e and in

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

## SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

compliance with the enclosure, mounting, spacing and segregation requirements of the ultimate application.

### 15. Essential Health and Safety Requirements:

The relevant EHSRs that have not been addressed by the standards listed in this certificate have been identified and assessed in the confidential report identified in item 8.

### 16. Test and Assessment Procedure and Conditions:

This Type Examination Certificate is the result of testing of a sample of the product submitted, in accordance with the provisions of the relevant specific standard(s), and assessment of supporting documentation. It does not imply an assessment of the whole production.

Whilst this certificate may be used in support of a manufacturer's claim for CE Marking, FM Approvals Europe Ltd accepts no responsibility for the compliance of the equipment against all applicable Directives in all applications.

This Certificate has been issued in accordance with FM Approvals Europe Ltd's ATEX Certification Scheme.

### 17. Schedule Drawings

A list of the significant parts of the technical documentation is annexed to this certificate and a copy has been kept by FM Approvals Europe Ltd.

### 18. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
15 October 2018	Original Issue.
18 February 2020	<u>Supplement 1:</u> Report Reference: RR222218 dated 17 <sup>th</sup> February 2020. Description of the Change: <ol style="list-style-type: none"><li>1. A correction of typographical errors in model code section and the electrical power ratings.</li><li>2. Certificate transferred from FM Approvals Ltd., notified body no. 1725, to FM Approvals Europe Ltd., notified body no. 2809</li><li>3. Update CDL</li></ol>
26 January 2021	<u>Supplement 2:</u> Report Reference: RR226270 dated 25 <sup>th</sup> January 2021. Description of the Change: Add digital interface and correct typo in model code to remove + for TC-MIDI fitted with 1 heat exchanger.

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

**SCHEDULE**  
to Type Examination Certificate No. FM18ATEX0012X

Date	Description
10 October 2024	<u>Supplement 3:</u> Report Reference: RR242035 dated 10 October 2024. Description of the Change(s): 1. Addition of product variants due to changes to electronics 2. EN 60079-0:2012+A11:2013 updated to EN IEC 60079-0:2018
6 December 2024	<u>Supplement 4:</u> Report Reference: RR243713 dated 5 December 2024. Description of the Change(s): Document Updates

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

## **ANNEX**

### **4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)**

#### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35  
h = Condensate drain; 00, 10 or 30  
j & k = Moisture detector/Filter; 00, 01, 10, or 11  
l = Status Outputs; 00 or 10  
n = Delta T control; 00 or 10

### **4496 211b2d1fg0000l0n0p TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchanger for H2/O2 applications)**

#### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1 or 2  
f, g = Heat exchanger; 10, 15, 10 or 15  
l = Status Outputs; 00 or 10  
n = Delta T control; 00 or 10  
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

### **4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)**

#### **Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35  
h = Condensate drain; 0, 2, or 4  
j & k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21, 22  
l = Status Outputs; 0 or 1  
n = Delta T control; 0 or 1

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**



### **4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)**

**Description of Equipment:**

b = Gas cooler model: 1 or 2  
d = Supply voltage; 1, 2 or 4  
f & g = Heat exchanger; 22, 27, 32 or 37  
h = Condensate drain; 0, 2, 4  
j & k = Moisture detector/Filter; 00, 01, 10, or 11  
l = Signal Outputs; 0 or 1  
n = no value assigned.

---

### **4496 311 b2defghijklmno TC-MIDI X2(fitted with 1 heat exchangers)**

**Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
e = Gas path; 1 or 2  
f,g = Heat exchangers; 10, 15, 20, 25, 30 or 35  
h = Condensate drain; 0, 1 or 3  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector/Filter; 00, 01, 10 or 11  
l,m = Signal output; 00 or 10  
n,o = Delta T control; 00 or 10

---

### **4496 311 b2defg0000lmnop TC-MIDI X2 (fitted with 1 heat exchangers for H2/O2 applications)**

**Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
e = Gas path; 1 or 2  
f,g = Heat exchangers; 10, 15, 60, 65  
l,m = Signal output; 00 or 10  
n,o = Delta T control; 00 or 10  
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**



**4496 312 b2d1fghijklm00 TC-MIDI + X2(fitted with 2 heat exchangers)**

**Description of Equipment:**

b = Gas cooler types 1 or 2  
d = Supply Voltage; 1 or 2  
f,g = Heat exchangers; 60, 65, 61, 66, 70, 75, 80 or 85  
h = Condensate drain; 0, 2, or 4  
i = Sample gas pumps; 0, 1, 2, 6, or 7  
j,k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21 or 22  
l,m = Signal outputs; 00 or 10  
n, o = Delta T Control; 00 or 10

---

**4496 611a2c1efghijkl000 TC-Double X2**

**Description of Equipment:**

a = Gas cooler types 1 or 2  
c = Voltage; 1 or 2  
e,f = Heat exchangers; 10, 15, 20, 25, 30 or 35  
g = Condensate drain; 0, 2, or 4  
h = Sample gas pumps; 0, 1, or 2  
i,j = Humidity sensor/Filter; 00, 01, 10, or 11  
k,l = Signal outputs; 00 or 10

---

**4496 611a2c1efghijkl000 TC-Double+ X2**

**Description of Equipment:**

a = Gas cooler types 1 or 2  
c = Voltage; 1 or 2  
e,f = Heat exchangers; 22, 27, 32, or 37  
g = Peristaltic pumps; 0, 2, or 4  
h = Sample gas pumps; 0, 1, or 2  
i,j = Moisture Detector/Filter; 00, 01, 10, or 11  
k,l = Status output; 00 or 10

---

**THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE**

# RMA-Formular und Erklärung über Dekontaminierung

## RMA-Form and explanation for decontamination



RMA-Nr./ RMA-No.

Die RMA-Nr. bekommen Sie von Ihrem Ansprechpartner im Vertrieb oder Service. Bei Rücksendung eines Altgeräts zur Entsorgung tragen Sie bitte in das Feld der RMA-Nr. "WEEE" ein./ You may obtain the RMA number from your sales or service representative. When returning an old appliance for disposal, please enter "WEEE" in the RMA number box.

Zu diesem Rücksendeschein gehört eine Dekontaminierungserklärung. Die gesetzlichen Vorschriften schreiben vor, dass Sie uns diese Dekontaminierungserklärung ausgefüllt und unterschrieben zurücksenden müssen. Bitte füllen Sie auch diese im Sinne der Gesundheit unserer Mitarbeiter vollständig aus./ This return form includes a decontamination statement. The law requires you to submit this completed and signed decontamination statement to us. Please complete the entire form, also in the interest of our employee health.

### Firma/ Company

Firma/ Company

Straße/ Street

PLZ, Ort/ Zip, City

Land/ Country

Gerät/ Device

Anzahl/ Quantity

Auftragsnr./ Order No.

### Ansprechpartner/ Person in charge

Name/ Name

Abt./ Dept.

Tel./ Phone

E-Mail

Serien-Nr./ Serial No.

Artikel-Nr./ Item No.

### Grund der Rücksendung/ Reason for return

- ☐ Kalibrierung/ Calibration ☐ Modifikation/ Modification  
☐ Reklamation/ Claim ☐ Reparatur/ Repair  
☐ Elektroaltgerät/ Waste Electrical & Electronic Equipment (WEEE)  
☐ andere/ other

bitte spezifizieren/ please specify

### Ist das Gerät möglicherweise kontaminiert?/ Could the equipment be contaminated?

- ☐ Nein, da das Gerät nicht mit gesundheitsgefährdenden Stoffen betrieben wurde./ No, because the device was not operated with hazardous substances.  
☐ Nein, da das Gerät ordnungsgemäß gereinigt und dekontaminiert wurde./ No, because the device has been properly cleaned and decontaminated.  
☐ Ja, kontaminiert mit:/ Yes, contaminated with:



☐  
explosiv/  
explosive



☐  
entzündlich/  
flammable



☐  
brandfördernd/  
oxidizing



☐  
komprimierte  
Gase/  
compressed  
gases



☐  
ätzend/  
caustic



☐  
giftig,  
Lebensgefahr/  
poisonous, risk  
of death



☐  
gesundheitsge-  
fährdend/  
harmful to  
health



☐  
gesund-  
heitsschädlich/  
health hazard



☐  
umweltge-  
fährdend/  
environmental  
hazard

### Bitte Sicherheitsdatenblatt beilegen!/ Please enclose safety data sheet!

Das Gerät wurde gespült mit:/ The equipment was purged with:

Diese Erklärung wurde korrekt und vollständig ausgefüllt und von einer dazu befugten Person unterschrieben. Der Versand der (dekontaminierten) Geräte und Komponenten erfolgt gemäß den gesetzlichen Bestimmungen.

This declaration has been filled out correctly and completely, and signed by an authorized person. The dispatch of the (decontaminated) devices and components takes place according to the legal regulations.

Falls die Ware nicht gereinigt, also kontaminiert bei uns eintrifft, muss die Firma Bühler sich vorbehalten, diese durch einen externen Dienstleister reinigen zu lassen und Ihnen dies in Rechnung zu stellen.

Should the goods not arrive clean, but contaminated, Bühler reserves the right, to commission an external service provider to clean the goods and invoice it to your account.

Firmenstempel/ Company Sign

Datum/ Date

rechtsverbindliche Unterschrift/ Legally binding signature



### **Vermeiden von Veränderung und Beschädigung der einzusendenden Baugruppe**

Die Analyse defekter Baugruppen ist ein wesentlicher Bestandteil der Qualitätssicherung der Firma Bühler Technologies GmbH. Um eine aussagekräftige Analyse zu gewährleisten muss die Ware möglichst unverändert untersucht werden. Es dürfen keine Veränderungen oder weitere Beschädigungen auftreten, die Ursachen verdecken oder eine Analyse unmöglich machen.

### **Umgang mit elektrostatisch sensiblen Baugruppen**

Bei elektronischen Baugruppen kann es sich um elektrostatisch sensible Baugruppen handeln. Es ist darauf zu achten, diese Baugruppen ESD-gerecht zu behandeln. Nach Möglichkeit sollten die Baugruppen an einem ESD-gerechten Arbeitsplatz getauscht werden. Ist dies nicht möglich sollten ESD-gerechte Maßnahmen beim Austausch getroffen werden. Der Transport darf nur in ESD-gerechten Behältnissen durchgeführt werden. Die Verpackung der Baugruppen muss ESD-konform sein. Verwenden Sie nach Möglichkeit die Verpackung des Ersatzteils oder wählen Sie selber eine ESD-gerechte Verpackung.

### **Einbau von Ersatzteilen**

Beachten Sie beim Einbau des Ersatzteils die gleichen Vorgaben wie oben beschrieben. Achten Sie auf die ordnungsgemäße Montage des Bauteils und aller Komponenten. Versetzen Sie vor der Inbetriebnahme die Verkabelung wieder in den ursprünglichen Zustand. Fragen Sie im Zweifel beim Hersteller nach weiteren Informationen.

### **Einsenden von Elektroaltgeräten zur Entsorgung**

Wollen Sie ein von Bühler Technologies GmbH stammendes Elektroprodukt zur fachgerechten Entsorgung einsenden, dann tragen Sie bitte in das Feld der RMA-Nr. „WEEE“ ein. Legen Sie dem Altgerät die vollständig ausgefüllte Dekontaminierungserklärung für den Transport von außen sichtbar bei. Weitere Informationen zur Entsorgung von Elektroaltgeräten finden Sie auf der Webseite unseres Unternehmens.

### **Avoiding alterations and damage to the components to be returned**

Analysing defective assemblies is an essential part of quality assurance at Bühler Technologies GmbH. To ensure conclusive analysis the goods must be inspected unaltered, if possible. Modifications or other damages which may hide the cause or render it impossible to analyse are prohibited.

### **Handling electrostatically conductive components**

Electronic assemblies may be sensitive to static electricity. Be sure to handle these assemblies in an ESD-safe manner. Where possible, the assemblies should be replaced in an ESD-safe location. If unable to do so, take ESD-safe precautions when replacing these. Must be transported in ESD-safe containers. The packaging of the assemblies must be ESD-safe. If possible, use the packaging of the spare part or use ESD-safe packaging.

### **Fitting of spare parts**

Observe the above specifications when installing the spare part. Ensure the part and all components are properly installed. Return the cables to the original state before putting into service. When in doubt, contact the manufacturer for additional information.

### **Returning old electrical appliances for disposal**

If you wish to return an electrical product from Bühler Technologies GmbH for proper disposal, please enter "WEEE" in the RMA number box. Please attach the fully completed decontamination declaration form for transport to the old appliance so that it is visible from the outside. You can find more information on the disposal of old electrical appliances on our company's website.

