



Refroidisseur de gaz de mesure

Série TC-Double X2

Manuel d'utilisation et d'installation

Notice originale





Bühler Technologies GmbH, Harkortstr. 29, D-40880 Ratingen
Tel. +49 (0) 21 02 / 49 89-0, Fax: +49 (0) 21 02 / 49 89-20
Internet: www.buehler-technologies.com
E-Mail: analyse@buehler-technologies.com

Veuillez lire attentivement le mode d'emploi avant d'utiliser l'appareil. Faites tout particulièrement attention aux indications d'avertissement et de sécurité. Dans le cas contraire, des risques sanitaires ou matériels peuvent apparaître. La responsabilité de Bühler Technologies GmbH est exclue pour toute modification de l'appareil effectuée par l'utilisateur ou toute utilisation non conforme.

Tous droits réservés. Bühler Technologies GmbH 2025

Information sur document

No. du document.....BF440022

Version..... 10/2024

Sommaire

1	Introduction	3
1.1	Utilisation conforme à la destination d'usage	3
1.2	Vue d'ensemble	3
1.3	Plaque signalétique	4
1.4	Contenu de la livraison	4
1.5	Indications de commande	5
1.5.1	TC-Double X2	5
1.5.2	TC-Double+ X2	6
2	Indications de sécurité	7
2.1	Indications importantes	7
2.2	Indications générales de risques	8
3	Transport et stockage	10
4	Assemblage et raccordement	11
4.1	Exigences quant au lieu d'installation	11
4.2	Montage	11
4.2.1	Raccordement capteur de débit (en option)	11
4.2.2	Branchement capteur d'humidité (option)	11
4.2.3	Branchement pompe péristaltique (option)	12
4.2.4	Raccordement des conduites de gaz de la pompe pour gaz de mesure (en option)	12
4.2.5	Raccordement échangeur de chaleur	12
4.2.6	Raccordement de dérivateur de condensat	13
4.3	Raccordements électriques	14
4.4	Sorties de signal	15
5	Fonctionnement et commande	16
5.1	Description des fonctions	16
5.2	Utilisation des fonctions de menu	17
5.2.1	Verrouillage de menu	17
5.2.2	Vue d'ensemble de guidage de menu	18
5.3	Description des fonctions de menu	20
5.3.1	Menu d'affichage	20
5.3.2	Menu principal	20
5.3.3	Sous-menu 1	21
5.3.4	Sous-menu 1 (réglages globaux)	22
5.3.5	Définir le menu favoriisé	25
6	Entretien	26
7	Entretien et réparation	27
7.1	Recherche de panne et résolution	27
7.1.1	Messages d'erreur sur l'écran	28
7.2	Indications de sécurité	29
7.3	Nettoyage et démontage de l'échangeur de chaleur	30
7.4	Changer le tuyau de la pompe péristaltique (option)	30
7.5	Changement de l'élément de filtre (option)	30
7.6	Séchage du capteur d'humidité (option)	31
7.7	Calibrage du capteur d'humidité (option)	31
7.8	Changement des valves d'admission et des soupapes d'échappement de la pompe pour gaz de mesure (en option)	31
7.9	Remplacement du joint torique de soupape by-pass (en option)	32
7.10	Changement du joint à soufflet (en option)	32
7.11	Pièces de rechange	33
7.11.1	Consommables et accessoires	33
8	Mise au rebut	34
9	Pièces jointes	35
9.1	Données techniques refroidisseur à gaz	35
9.2	Caractéristiques techniques options	35

9.3	Schéma de procédé	36
9.4	Courbes de puissance.....	37
9.5	Échangeur thermique	37
9.5.1	Description échangeur de chaleur	37
9.5.2	Vue d'ensemble de l'échangeur thermique	38
9.6	Dimensions (mm)	39
10	Documents joints	40

1 Introduction

1.1 Utilisation conforme à la destination d'usage

Cet appareil est conçu pour un usage dans des systèmes d'analyse de gaz. Il constitue une composante essentielle à la préparation du gaz de mesure pour protéger l'appareil de l'humidité résiduelle dans le gaz de mesure.

Le matériel peut être utilisé dans une atmosphère de gaz explosive de la zone 2, classe d'explosion IIC (ATEX, IECEx et EAC Ex), qui est rarement et, le cas échéant, que brièvement explosive, et dans la classe I, division 2 (US et Canada).

Le montage optionnel de divers appareils supplémentaires peut limiter la plage d'utilisation de l'appareil.

Refroidisseur avec certificat pour le Canada et IECEx

Le matériel d'exploitation doit être monté dans un boîtier IP54 ne pouvant être ouvert qu'à l'aide d'un outil.

Refroidisseur avec certificat pour les USA

Le matériel d'exploitation doit être monté dans un boîtier IP54 ne pouvant être ouvert qu'à l'aide d'un outil conçu pour abriter une ou plusieurs méthodes de câblage de Class I Division 2 selon le National Electric Code (ANSI/NFPA 70).

Refroidisseur avec certificat pour ATEX

L'appareil doit être installé dans un boîtier ne pouvant être ouvert qu'à l'aide d'un outil, présentant au moins le degré de protection IP54 et répondant aux exigences de la norme EN 60079-0 ou certifié Ex e, et satisfaisant aux exigences de l'application finale en matière de boîtier, d'assemblage, d'espacement et de séparation.

Refroidisseur avec certificat EAC Ex

Le matériel doit être monté dans un boîtier doté d'un indice de protection IP54 et satisfaisant aux exigences de la norme GOST 14254-2015.

Veuillez respecter les indications de la fiche technique concernant la finalité spécifique, les combinaisons de matériaux présentes ainsi que les limites de pression et de température.

1.2 Vue d'ensemble

La série TC-Double X2 a été spécialement conçue pour de hautes capacités de refroidissement, de hautes températures ambiantes et un refroidissement en deux opérations pour minimiser les effets de dispersion. Avec le dispositif TC-Double+ X2, les deux températures du bloc de refroidissement peuvent être réglées indépendamment l'une de l'autre.

Une autre application de ce refroidisseur se trouve dans la variante avec pré-refroidisseur passif intégré, cela signifie que la première étape du refroidissement n'est pas pilotée électroniquement.

Les dispositifs de refroidissement de Peltier sont divisés selon la puissance de refroidissement ou la température raisonnable d'environnement. Ce classement se retrouve dans la désignation de type. Le numéro d'article précis du type que vous avez défini est déterminé à partir du code dans la rubrique Indications de commande.

Utilisation		Utilisations standards	
Température de fonctionnement	40 °C	50 °C	
2 échangeurs thermiques en série	TC-Double 6111 X2 :	TC-Double 6112 X2 :	
2 échangeurs thermiques en série	TC-Double+ 6111 X2 :	TC-Double+ 6112 X2 :	

D'autres composants devant être présents dans tous les systèmes de préparation peuvent être intégrés en option :

- Pompe péristaltique pour la dérivation de condensat
- Filtre,
- Capteur d'humidité,
- Pompe de gaz de mesure.

Avec ses options, le refroidisseur dispose ainsi une grande variété de configuration. Cette rubrique décrit comment simplifier à moindres frais la réalisation d'un système complet en utilisant des composants pré-montés et équipés de flexibles. En outre, nous avons pris soin de garantir une bonne accessibilité des consommables et des pièces d'usure.

1.3 Plaque signalétique

Exemple :

Fabricant avec adresse	→	 Technologies GmbH Harkortstr.29, D-40880 Ratingen	
Désignation de type et tension	→	TC-Double 230 V, 50/60Hz, 390W	
n° de série, n° d'article	→	101001081115 44966112121115000000	
identifications de protection contre allumage (Atex, IECex et US/Canada)	→	FM18ATEX0012X II 3 G Ex ec nC IIC T4 Gc IECEX FMG 18.0005X Ex ec nC IIC T4 Gc USA/Canada: CL I DIV 2 GP ABCD	 
numéro de validation EAC Ex	→	RU C-DE.HA65.B.00608/20	
Description	→	0°C...60°C	
Année de fabrication	→	02/2024	
		BX440022 	

1.4 Contenu de la livraison

- Refroidisseur
- Documentation produit
- Accessoires de raccordement ou de montage (en option)

1.5 Indications de commande

1.5.1 TC-Double X2

Le numéro d'article codifie la configuration de votre appareil. Utilisez pour cela les codes types suivants :

4496	6	1	1	X	2	X	1	X	X	X	X	X	X	0	0	0	0	Caractéristique du produit
Type de refroidisseur de gaz																		
1																		TC-Double 6111 X2 : Température ambiante 40 °C
2																		TC-Double 6112 X2 : Température ambiante 60 °C
Autorisation																		
2																		pour les zones à risque d'explosion
Tension d'alimentation																		
1																		115 V AC, 50/60 Hz
2																		230 V AC, 50/60 Hz
Échangeur thermique																		
1	1	0																Acier inoxydable, PTS, métrique
1	1	5																Acier inoxydable, PTS-I, en pouces
1	2	0																Verre Duran, PTG, métrique
1	2	5																Verre Duran, PTG-I, en pouces
1	3	0																PVDF, PTV, métrique
1	3	5																PVDF, PTV-I, en pouces
Dérivation de condensat ¹⁾																		
0																		sans dérivation de condensat
2																		CPdouble X2 avec raccords de tuyau, coudé
4																		CPdouble X2 avec raccords vissés ²⁾
Pompes pour gaz de mesure ^{1) 3)}																		
0																		sans pompe pour gaz de mesure
1																		P1.3, PVDF
2																		P1.3, avec soupape by-pass
Capteur d'humidité/filtre ^{1) 2)}																		
0	0																	sans filtre, sans capteur d'humidité
0	1																	sans filtre, 1 capteur d'humidité avec adaptateur PVDF ⁴⁾
1	0																	1 filtre, sans capteur d'humidité
1	1																	1 filtre avec capteur d'humidité intégré
Sorties de signal																		
0	0																	sortie d'état uniquement
1	0																	Sortie analogique, 4...20 mA en outre

¹⁾ Lorsque l'option est sélectionnée, la température ambiante maximale est limitée à 50 °C.

²⁾ Raccordement métrique, voire en pouces, selon l'échangeur thermique.

³⁾ Tubulure d'usine pour fonctionnement en aspiration.

⁴⁾ Aussi disponible en acier inoxydable.

1.5.2 TC-Double+ X2

Le numéro d'article codifie la configuration de votre appareil. Utilisez pour cela les codes types suivants :

4496	6	1	1	X	2	X	1	X	X	X	X	X	X	0	0	0	0	Caractéristique du produit
Type de refroidisseur de gaz																		
1																	TC-Double+ 6111 X2 : Température ambiante 40 °C	
2																	TC-Double+ 6112 X2 : Température ambiante 60 °C	
Autorisation																		
2																	pour les zones à risque d'explosion	
Tension d'alimentation																		
1																	115 V AC, 50/60 Hz	
2																	230 V AC, 50/60 Hz	
Échangeur thermique																		
1	2	2															Verre Duran, PTG-2, métrique	
1	2	7															Verre Duran, PTG-2-I, en pouces	
1	3	2															PVDF, PTV-2, métrique	
1	3	7															PVDF, PTV-2-I, en pouces	
Dérivation de condensat ¹⁾																		
0																	sans dérivation de condensat	
2																	CPdouble X2 avec raccords de tuyau, coudé	
4																	CPdouble X2 avec raccords vissés ²⁾	
Pompes pour gaz de mesure ^{1) 3)}																		
0																	sans pompe pour gaz de mesure	
1																	P1.3, PVDF	
2																	P1.3, avec soupape by-pass	
Capteur d'humidité/filtre ^{1) 2)}																		
0	0																sans filtre, sans capteur d'humidité	
0	1																sans filtre, 1 capteur d'humidité avec adaptateur PVDF ⁴⁾	
1	0																1 filtre, sans capteur d'humidité	
1	1																1 filtre avec capteur d'humidité intégré	
Sorties de signal																		
0	0																sortie d'état uniquement	
1	0																Sortie analogique, 4...20 mA en outre	

¹⁾ Lorsque l'option est sélectionnée, la température ambiante maximale est limitée à 50 °C.

²⁾ Raccordement métrique, voire en pouces, selon l'échangeur thermique.

³⁾ Tubulure d'usine pour fonctionnement en aspiration.

⁴⁾ Aussi disponible en acier inoxydable.

2 Indications de sécurité

2.1 Indications importantes

INDICATION



Cet appareil peut être utilisé dans des espaces à risque d'explosion.

L'utilisation de l'appareil n'est autorisée que si :

- le produit est utilisé dans les conditions décrites dans les instructions de service et d'installation, pour une utilisation conforme aux indications de la plaque signalétique et pour les applications pour lesquelles il est conçu. Dans le cas de modifications propres de l'appareil, toute responsabilité de la part de Bühler Technologies GmbH est exclue,
- les indications et dénominations sur les plaques signalétiques sont respectées,
- les valeurs limites dans la fiche technique et le mode d'emploi sont respectées,
- les dispositifs de surveillance / le dispositif de protection sont correctement raccordés,
- les travaux de maintenance et de réparation non décrits dans ce mode d'emploi sont effectués par Bühler Technologies GmbH,
- des pièces de rechange originales sont utilisées.

L'installation d'équipements électriques dans des zones à risque d'explosion nécessite de respecter les prescriptions nationales suivantes :

- IEC/EN 60079-14
- National electric code (NEC)
- Canadian electric code (CEC)

Les directives nationales supplémentaires concernant la mise en service, l'exploitation, l'entretien, la maintenance et la mise au rebut doivent être respectées.

Cette instruction d'utilisation fait partie du moyen de production. Le fabricant se réserve le droit de modifier sans préavis toute donnée relative aux performances, aux spécifications ou à l'interprétation. Conservez ces instructions d'utilisation pour une utilisation ultérieure.

Mots-signaux pour avertissements

DANGER

Mot-signal pour désigner une menace à haut risque entraînant immédiatement la mort ou des blessures corporelles lourdes si elle n'est pas évitée.

AVERTISSEMENT

Mot-signal pour désigner une menace de risque intermédiaire pouvant entraîner la mort ou des blessures corporelles lourdes si elle n'est pas évitée.

ATTENTION

Mot-signal pour désigner une menace à faible risque pouvant entraîner des dommages matériels ou des blessures corporelles légères à moyennement graves si elle n'est pas évitée.

INDICATION

Mot-signal pour une information importante à propos du produit, information à laquelle il faudrait accorder une attention importante.

Signaux d'avertissement

Ce mode d'emploi utilise les signaux d'avertissement suivants :



Signal d'avertissement général



Signal d'obligation général



Avertissement de tension électrique



Débrancher la fiche d'alimentation



Avertissement d'inhalation de gaz toxiques



Porter une protection respiratoire



Avertissement de liquides irritants



Porter une protection faciale



Avertissement de risque d'explosion



Porter des gants



Avertissement de surface chaude

2.2 Indications générales de risques

L'appareil ne doit être installé que par du personnel spécialisé et familiarisé avec les exigences de sécurité et les risques.

Respectez impérativement les indications de sécurité pertinentes relatives au lieu d'installation ainsi que les règles techniques en vigueur. Évitez les défaillances et les dommages corporels et matériels.

L'exploitant de l'installation doit s'assurer que :

- les indications de sécurité et les instructions d'utilisation sont disponibles et respectées,
- les directives nationales respectives de prévention des accidents sont respectées,
- les données et conditions d'utilisation licites sont respectés,
- les dispositifs de protection sont utilisés et les travaux d'entretien prescrits effectués,
- les réglementations légales pour la mise au rebut sont respectées,
- les prescriptions d'installation nationales en vigueur sont respectées.

Entretien, réparation

Lors de toute opération de maintenance et de réparation, respecter les points suivants :

- Les réparations sur les outils d'exploitation doivent être uniquement effectuées par le personnel autorisé par Bühler.
- Réalisez exclusivement les travaux de modification, de maintenance ou de montage décrits dans ces instructions de commande et d'installation.
- N'utilisez que des pièces de rechange originales.
- Ne pas utiliser de pièces de rechange endommagées ou défectueuses. Avant le montage, effectuez le cas échéant un contrôle visuel afin de détecter les dommages évidents sur les pièces de rechange.

Lorsque des travaux de maintenance de toutes sortes sont effectués, les dispositions de sécurité et d'exploitation applicables du pays d'utilisation doivent être respectées.

DANGER

Tension électrique

Danger d'électrocution



- Pour tous travaux, débranchez l'appareil du réseau.
- Assurez-vous que l'appareil ne puisse pas redémarrer involontairement.
- L'appareil ne peut être ouvert que par des personnels spécialisés qualifiés et instruits.
- Veillez à ce que l'alimentation électrique soit correcte.



DANGER



Gaz/condensats toxiques et irritants

Le gaz de mesure/les condensats peuvent être nocifs pour la santé.

- a) Le cas échéant, assurez une évacuation sûre du gaz/des condensats.
- b) Coupez l'arrivée de gaz lors de tous travaux d'entretien et de réparation.
- c) Lors des travaux d'entretien, protégez-vous des gaz/condensats toxiques/irritants. Portez l'équipement de protection approprié.



DANGER



Danger d'explosion

Danger mortel et danger d'explosion par fuite de gaz en cas d'utilisation non conforme.

- a) N'utilisez l'appareil que comme décrit dans ces instructions.
- b) Respectez les conditions de processus.
- c) Vérifiez l'étanchéité des tuyaux.

AVERTISSEMENT



Risque de rupture

- a) Protégez l'appareil des chocs externes.
- b) Mettez l'appareil à l'abri de chutes d'objets.

3 Transport et stockage

Les produits doivent toujours être transportés dans leur emballage d'origine ou dans un emballage de remplacement approprié. En cas de non utilisation, les matériels d'exploitation doivent être protégés de l'humidité et de la chaleur. Ils doivent être stockés dans une pièce couverte, sèche et sans poussière à une température comprise entre - 20°C et 60°C (- 4 °F à 140 °F).

4 Assemblage et raccordement

4.1 Exigences quant au lieu d'installation

L'appareil est destiné à un montage mural dans des lieux fermés. En cas d'utilisation en plein air, une protection contre les intempéries suffisante doit être prévue.

Montez l'appareil de sorte à laisser assez d'espace sous le refroidisseur pour dériver le condensat. Un peu d'espace doit également être prévu au-dessus pour l'alimentation en gaz.

Il faut veiller à ce que les limites autorisées de température ambiante soient respectées. La convection du refroidisseur ne doit pas être entravée. Un espace suffisant doit être laissé entre les ouvertures de ventilation et l'obstacle le plus proche. En particulier du côté de l'évacuation de l'air, une distance minimale de 10 cm doit être assurée.

Lors du montage dans des boîtiers fermés, par exemple dans des armoires d'analyse, veuillez assurer une ventilation suffisante. Si la convection ne suffit pas, nous recommandons de rincer l'armoire à l'air ou de prévoir un ventilateur afin d'abaisser la température interne.

4.2 Montage

Installez l'alimentation en gaz vers le refroidisseur avec une inclinaison. Les entrées de gaz sont marquées en rouge et comportent la mention « IN ».

En cas de grosses formations de condensat, nous recommandons de placer un séparateur de liquides avec purge automatique de condensat.

Pour la dérivation du condensat, des récipients en verre et un purgeur sont disponibles et doivent être montés à l'extérieur, sous l'appareil. En cas d'utilisation de purgeurs de condensat automatiques, la pompe pour gaz de mesure doit être montée en amont du refroidisseur (fonctionnement sous pression). Dans le cas contraire, le bon fonctionnement du purgeur de condensat n'est pas assuré.

Si la pompe pour gaz de mesure se trouve à la sortie du refroidisseur (aspiration), l'utilisation de récipients collecteurs de condensat ou de pompes péristaltiques est recommandée.

4.2.1 Raccordement capteur de débit (en option)

Si le refroidisseur est commandé avec l'**option capteur d'humidité sans filtre**, il est monté en usine dans un adaptateur de débit.

La liaison entre la sortie d'échangeur thermique et l'entrée d'adaptateur de débit n'est pas globalement pourvue de tuyaux. Le raccordement G1/4 ou NPT 1/4" (adaptateur de débit marqué de NPT) pour l'entrée/la sortie de gaz doit être branché avec précaution et de manière appropriée avec des raccords filetés adaptés. Le sens de l'écoulement n'est alors pas important.

4.2.2 Branchement capteur d'humidité (option)

Si le refroidisseur est commandé avec l'**option capteur d'humidité**, il est déjà monté en usine dans un adaptateur de débit, ou pour l'**option filtre**, est raccordé et monté dans la tête du filtre.

4.2.3 Branchement pompe péristaltique (option)

Si vous avez commandé le refroidisseur avec une pompe péristaltique montée, celle-ci est déjà installée et câblée à la livraison. Les échangeurs thermiques commandés en même temps sont montés et branchés à la pompe péristaltique.

Le raccordement via les assemblages vissés de la sortie de condensat de la pompe doit être fait en utilisant le flexible adéquat, prudemment et de manière appropriée.

INDICATION



L'installation de **pompes** péristaltiques CPsingle / CPdouble limite la **pression de fonctionnement** maximale du système !
Pression de fonctionnement ≤ 1 bar

4.2.4 Raccordement des conduites de gaz de la pompe pour gaz de mesure (en option)

Si vous avez commandé le refroidisseur avec une pompe pour gaz de mesure montée, celle-ci est déjà installée raccordée et câblée à la livraison. Les pièces commandées en même temps sont montées et branchées aux pompes pour gaz de mesure.

Évitez les installations mixtes, c'est-à-dire des conduites tubulaires métalliques sur des corps en plastique. Si cela est inévitable pour certaines utilisations, vissez les raccords filetés métalliques dans le corps de pompe avec précaution et sans jamais forcer.


Posez les conduites tubulaires de manière à ce que la conduite à l'entrée/la sortie reste élastique sur une distance suffisante.


Les pompes sont caractérisées sur la bague de fixation par **IN** pour Inlet (admission) et **OUT** pour Outlet (évacuation). Assurez-vous que les raccords sur les conduites de gaz sont bien étanches.

4.2.5 Raccordement échangeur de chaleur

Pour minimiser les effets de dispersion du gaz dans le refroidisseur, les deux échangeurs de chaleur (de construction identique) doivent fonctionner en série l'un derrière l'autre. Pour cela, la procédure suivante devrait être suivie :

1. Ligne d'entrée de gaz sur l'entrée de gaz de l'échangeur de chaleur identifiée en rouge n° 2 (refroidissement préalable).
2. Ligne de raccordement entre la sortie de gaz de l'échangeur de chaleur n° 2 et l'entrée de gaz identifiée en rouge de l'échangeur de chaleur n° 1 (refroidissement subséquent).
3. Montage de la ligne terminale de sortie du gaz à la sortie du gaz de l'échangeur de chaleur n° 1.

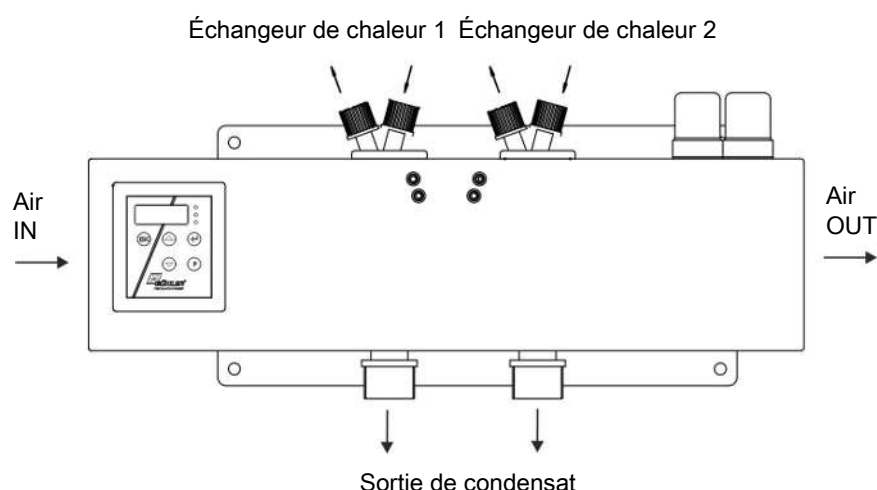


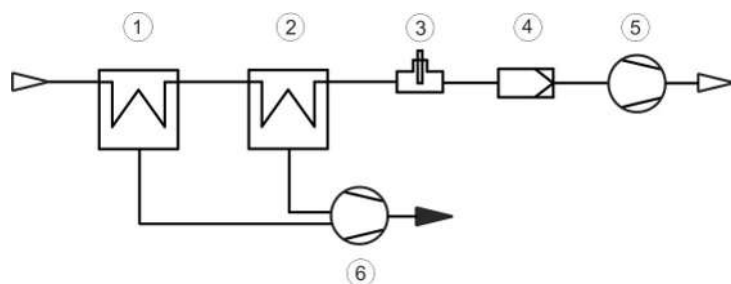Organigramme :

1 Échangeur de chaleur 2 /refroidissement préalable	4 Filtre (en option)
2 Échangeur de chaleur 1 /refroidissement subséquent	5 Pompe pour gaz de mesure (en option)
3 Capteur d'humidité (en option)	6 Pompe de condensat (en option)

Les entrées de gaz sont identifiées en rouge.

Dans le cas d'échangeurs de chaleur en verre, il est nécessaire de faire attention au bon positionnement du joint d'étanchéité lors du raccordement des conduites de gaz (voir illustration). Le joint se compose d'un anneau en silicone avec une face en PTFE. Le côté en PTFE doit être orienté vers le filetage en verre.

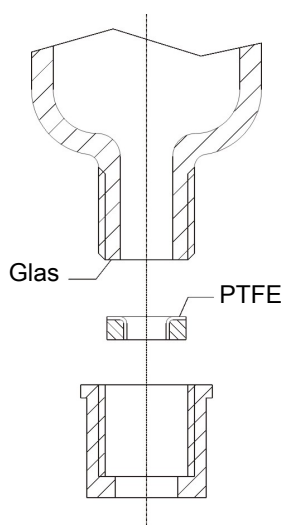

Dans le cas d'échangeurs thermiques en acier inoxydable, il convient de tenir compte de l'ouverture de clé compatible avec la sélection de raccords vissés.

Raccordements de gaz PTS/PTS-I : SW 14 ou 9/16

Vidange de condensat PTS/PTS-I : SW 22

4.2.6 Raccordement de dérivateur de condensat

Selon le matériau, il est nécessaire d'établir une conduite de raccordement entre l'échangeur thermique et le dérivateur de condensat en utilisant des raccords vissés et des tubes ou tuyaux. En cas d'acier inoxydable, il est possible d'accrocher le dérivateur de condensat directement sur le tube de raccordement. Pour les tuyaux, le dérivateur de condensat doit être attaché séparément à l'aide d'un collier de serrage.

Le dérivateur de condensat peut être directement fixé sur l'échangeur thermique.

Les conduites de condensat doivent en général être montées avec une inclinaison et une section nominale minimale de DN 6/8 (1/4").

4.3 Raccordements électriques

L'exploitant doit installer pour l'appareil un dispositif de séparation externe étant attribué à cet appareil de manière reconnaissable.

Ce dispositif de séparation

- doit se trouver à proximité de l'appareil,
- doit être facilement accessible pour l'utilisateur,
- doit satisfaire aux normes IEC 60947-1 et IEC 60947-3,
- doit séparer tous les conducteurs de courant du raccordement d'alimentation et de la sortie d'état et
- ne doit pas être intégré dans la ligne d'alimentation.

La ligne d'alimentation de l'appareil doit être sécurisée selon les indications présentes dans les données techniques.

Liaison équipotentielle / charge électrostatique

Les charges électrostatiques peuvent provoquer la formation d'étincelles pouvant s'enflammer. Évitez les charges électrostatiques. Toutes les pièces conductrices du refroidisseur doivent être reliées à la terre !

Une connexion pour un fil de mise à la terre / liaison équipotentielle est installée sur le boîtier. Assurez-vous que le boîtier dispose d'une mise à la terre suffisante (section minimum du conducteur 4 mm²).

Respectez en particulier les exigences de EN 60079-14 !

AVERTISSEMENT

Tension dangereuse



Le raccordement ne peut être entrepris que par des personnels formés et qualifiés.

ATTENTION

Tension erronée du réseau



Une tension de réseau erronée peut détruire l'appareil.

Lors du raccordement, faire attention à ce que la tension du réseau soit correcte conformément à la plaque signalétique.

AVERTISSEMENT

Haute tension



Endommagement de l'appareil lors du contrôle de l'isolation

N'effectuez **pas de contrôle de rigidité diélectrique avec une haute tension** sur l'ensemble de l'appareil !

Essai de résistance diélectrique

Cet appareil est équipé de protections CEM importantes. Les contrôles nécessaires ont été effectués à l'usine (tension de test selon l'élément 2,1 kV ou 2,55 kV DC).


Si vous voulez effectuer vous-même encore une fois un contrôle de rigidité diélectrique, vous pouvez l'effectuer sur l'appareil entier. Vérifiez l'appareil uniquement avec les valeurs prédéterminées et avec la tension continue. Un contrôle de la rigidité diélectrique avec courant alternatif peut endommager les composants électroniques. La tension recommandée est de 2,1 kV DC, 2 s. Avant l'essai, retirez toutes les lignes d'alimentation de l'appareil. La tension peut être appliquée directement par l'intermédiaire du raccordement au réseau.

Raccordement via connecteur


L'appareil est équipé d'une fiche selon EN 175301-803 et destinée à l'alimentation en tension et à la sortie de signal. Elles doivent être placées de manière à éviter toute confusion lorsque le raccordement de conduite est correct. Pour cette raison, veillez à ce que les fiches soient de nouveau assemblées en conformité après le raccordement des conduites. Les affectations de raccordement sont indiquées comme suit, les numéros correspondant aux numéros sur les fiches :

Les sections de ligne doivent être ajustées au courant de mesure. Utilisez au maximum une section de câble de 1,5 mm² (AWG 16) et un diamètre de câble de 8 à 10 mm (0,31 - 0,39 pouces).


Numérotation de fiche




Raccordement secteur S1



Sortie d'état S2 *



Sortie analogique S3

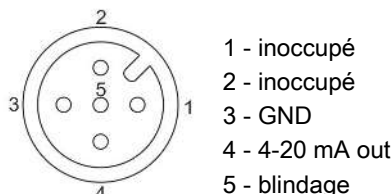

* En cas d'utilisation du contact d'alarme sous tension ≥ 33 V AC ou 70 V DC, le conducteur de protection (PE) doit être raccordé. Les zones de serrage de S1 et S2 ont un diamètre de 8-10 mm (0,31 - 0,39 pouces).

4.4 Sorties de signal

L'appareil est équipé de différents signaux d'état. La capacité de commutation maximale des sorties d'alarme est de 250 V AC/ 150 V DC, 2 A, 50 VA chacune.

Une alarme est déclenchée par le biais de la sortie d'état (S2) lorsque la température dans le bloc 1 se situe en dehors des valeurs limites fixées. Il n'est cependant pas signalé si l'alarme a été déclenchée pour cause de sur-température ou de sous-température.

Description des sorties de signal

	Fonction/Type de contact	Description
Vers S2)	Contact d'inverseur interne : max. 250 V AC/150 V DC, 2 A, 50 VA	deux sorties de commutation permettent de signaler les états d'appareil suivants : Contact fermé entre 3 et 2 (alarme) – Pas de tension secteur et/ou valeur réelle de température en dehors des seuils d'alerte définis Contact fermé entre 3 et 1 (ok) – Tension secteur appliquée + valeur réelle de température en dehors des seuils d'alerte définis
Vers S3)	4-20 mA sortie analogue ($R_{charge} < 500 \Omega$)	Signalisation de la température réelle dans le bloc 1 (veuillez utiliser un câble blindé) $T_{Refroidisseur} = -20 \text{ °C} \triangleq (-4 \text{ °F}) \rightarrow 4 \text{ mA} / 2 \text{ V}$ $T_{Refroidisseur} = 5 \text{ °C} \triangleq (41 \text{ °F}) \rightarrow 9 \text{ mA} / 4,5 \text{ V}$ $T_{Refroidisseur} = 60 \text{ °C} \triangleq (140 \text{ °F}) \rightarrow 20 \text{ mA} / 10 \text{ V}$

Le panneau avant du module d'affichage contient trois LED :

Couleur	Libellé	Fonction
Rouge	S2	Température excessive / insuffisante Défaillance de l'appareil
Jaune	S1	Réservé
Vert	OP	Fonctionnement normal

Les LED OP et S2 signalisent l'état de l'appareil analogue au S2.

Si l'option „signal de température“ est intégrée, le signal pour la température réelle à la sortie analogue du refroidisseur est disponible.

Le signal de température peut être baissé via la fiche à encastrer (S3) avec le raccord M12x1. Ce connecteur se trouve à côté des raccordements de la sonde d'humidité sur la partie supérieure du refroidisseur.

La température affichée en continu sur le display (CH1) correspond à la température dans le bloc 1 (refroidissement subséquent). Le signal analogue de température correspond également à la température dans le bloc 1.

5 Fonctionnement et commande

INDICATION



L'appareil ne doit pas être exploité en dehors du cadre de ses spécifications !

Après mise en marche du refroidisseur, la température du bloc s'affiche (bloc 1). L'affichage clignote jusqu'à ce que la température de bloc ait atteint la valeur de consigne réglée ($\pm$ la plage d'alarme réglable). Le contact d'état est en position d'alarme.

Si la plage de température de consigne est atteinte, la température est indiquée de manière permanente et le contact d'état commute.

Si, lors du fonctionnement, l'affichage clignote ou bien si un message d'erreur apparaît, veuillez consulter le chapitre « Recherche et élimination des pannes ».

Les données de performance et limites doivent être prises dans la fiche technique.

5.1 Description des fonctions

La commande du refroidisseur s'effectue via un microprocesseur. Le pré-réglage d'usine prend en compte les différentes caractéristiques des échangeurs de chaleur intégrés dès la commande.

L'écran programmable représente la température de bloc selon l'unité d'affichage sélectionnée ($^{\circ}\text{C}$ / $^{\circ}\text{F}$) ($^{\circ}\text{C}$ en usine). 5 touches de commande de menu permettent d'actionner simplement les réglages individuels des applications. Cela concerne d'une part le point de rosée de consigne pouvant être réglé de 2°C (36 à 68°F) à 20°C (réglage d'usine 5°C / 41°F).

D'autre part, les seuils d'alerte de sous-température et sur-température peuvent être réglés. Ceux-ci sont réglés par rapport au point de rosée réglé T_a .

Pour la sous-température, une plage de $T_a - 1$ jusqu'à $- 3 \text{ K}$ (au moins 1°C / 34°F de température de bloc de refroidissement) est disponible, une plage de $T_a + 1$ jusqu'à $+ 7 \text{ K}$ est disponible pour le réglage d'usine. Les réglages d'usine pour les deux valeurs sont 3 K .

Le clignotement de l'affichage et le relais d'état signalent un dépassement par le haut ou par le bas de la plage d'avertissement réglée (par ex. après allumage).

La sortie d'état peut par ex. être utilisée pour commander la pompe de gaz de mesure, afin de permettre d'enclencher le flux de gaz dès que la plage de refroidissement est atteinte ou pour éteindre la pompe si l'alarme du capteur d'humidité s'enclenche.

Le condensat collecté peut être évacué via des pompes péristaltiques ou le dérivateur de condensat automatique intégré.

De plus, il est également possible d'utiliser des filtres fins dans lesquels des capteurs d'humidité peuvent être intégrés, en option cependant.

La cloche en verre permet de voir les salissures de l'élément filtrant.

Le capteur d'humidité peut être démonté facilement. Cela peut être nécessaire si du condensat devait pénétrer dans le refroidisseur du fait d'une panne et ne pouvait plus être transporté par la pompe péristaltique, ou le dérivateur de condensat automatique.

Le TC-Double est équipé d'une autre étape de refroidissement qui est utilisée pour le pré-refroidissement du gaz (échangeur de chaleur 2), dont la température de bloc dépend de la température ambiante et de la charge. La valeur cible de l'étape de pré-refroidissement correspond à celle du dem bloc 1.

5.2 Utilisation des fonctions de menu

Explication courte du principe de commande :

La commande s'effectue au moyen de 5 touches. Elles possèdent les fonctions suivantes :

Touche	Plage	Fonctions
← ou OK	Affichage	– Passage de l'affichage de la valeur mesurée au menu principal
	Menu	– Sélection du point de menu affiché
	Saisie	– Acceptation d'une valeur éditée ou d'une sélection
▲	Affichage	– passage temporaire à un affichage de valeur de mesure alternative (si option disponible)
	Menu	– Défiler vers l'arrière
	Saisie	– Augmenter la valeur ou naviguer dans la sélection – valable ici : – Presser 1 fois la touche = modifier le paramètre / la valeur d'un incrément ; – Maintenir la touche pressée = déroulement rapide (uniquement pour les valeurs numériques) – L'affichage clignote : paramètre / valeur modifié(e) – L'affichage ne clignote pas : paramètre / valeur d'origine
▼	Affichage	– passage temporaire à un affichage de valeur de mesure alternative (si option disponible)
	Menu	– Défiler vers l'avant
	Saisie	– Diminuer la valeur ou naviguer dans la sélection
ESC	Menu	– Revenir vers le niveau supérieur
	Saisie	– Revenir au menu Les modifications ne sont pas sauvegardées !
F ou Func		– Définition d'un menu favorisé. (remarque : Le menu favorisé est également appelé même en cas de verrouillage de menu actif !)

5.2.1 Verrouillage de menu

Afin d'éviter toute modification non intentionnelle des réglages de l'appareil, certains menus peuvent être verrouillés. Un code doit pour ceci être défini. Pour savoir comment mettre en place le verrouillage de menu voire l'annuler, consulter « Réglages globaux » dans le menu (LOP) au point de menu LOP > LDC.

Lors de la livraison, le verrouillage de menu **n'est pas** actif et tous les points de menu sont accessibles.

En cas de verrouillage de menu actif, uniquement les points de menu suivants sont visibles si le code correct n'a pas été saisi :

Point de menu	Explication
LOP > uni L	Sélection de l'unité de température affichée (°C ou °F).
F ou Func.	Accès au menu favorisé
INDICATION! Ce menu peut provenir du domaine normalement verrouillé.	

5.2.2 Vue d'ensemble de guidage de menu

Si vous pressez le touche **OK** en fonctionnement normal, la demande de saisie **LoDE** apparaît sur l'afficheur en cas de verrouillage de menu actif. Saisissez le code correct au moyen des touches **▲** et **▼** et pressez **OK**.

En cas de saisie erronée ou en cas de non saisie, le verrouillage de menu n'est pas levé et vous n'avez pas accès à tous les points de menu.

Si vous avez oublié le mot de passe, vous pouvez accéder à tout moment au menu à l'aide du code maître 287 et le verrouillage de menu est désactivé.


La vue d'ensemble de la structure de menu est présentée sur la figure suivante.

Les points entourés en pointillés ne sont affichés que si les réglages correspondants ont été effectués, voire uniquement si des messages d'état sont présents.

Les réglages en usine standards et les plages de réglage sont indiqués dans la vue d'ensemble ainsi qu'au point de menu respectif. Les réglages en usine standards sont valables tant qu'aucune autre décision n'a été prise.


Vous pouvez interrompre les saisies et la sélection de menu, sans sauvegarde, à l'aide de la touche **ESC**.

Menu :




1. Désignation de menu
2. Affichage
3. Explication brève

Paramètre :




4. Saisie d'une valeur
5. Réglages d'usine
6. Plage de paramètres



7. Sélection dans une liste de valeurs
8. Réglages d'usine
9. Plage de paramètres / Sélection

Guidage de menu en option :



10. boîte hachurée = option

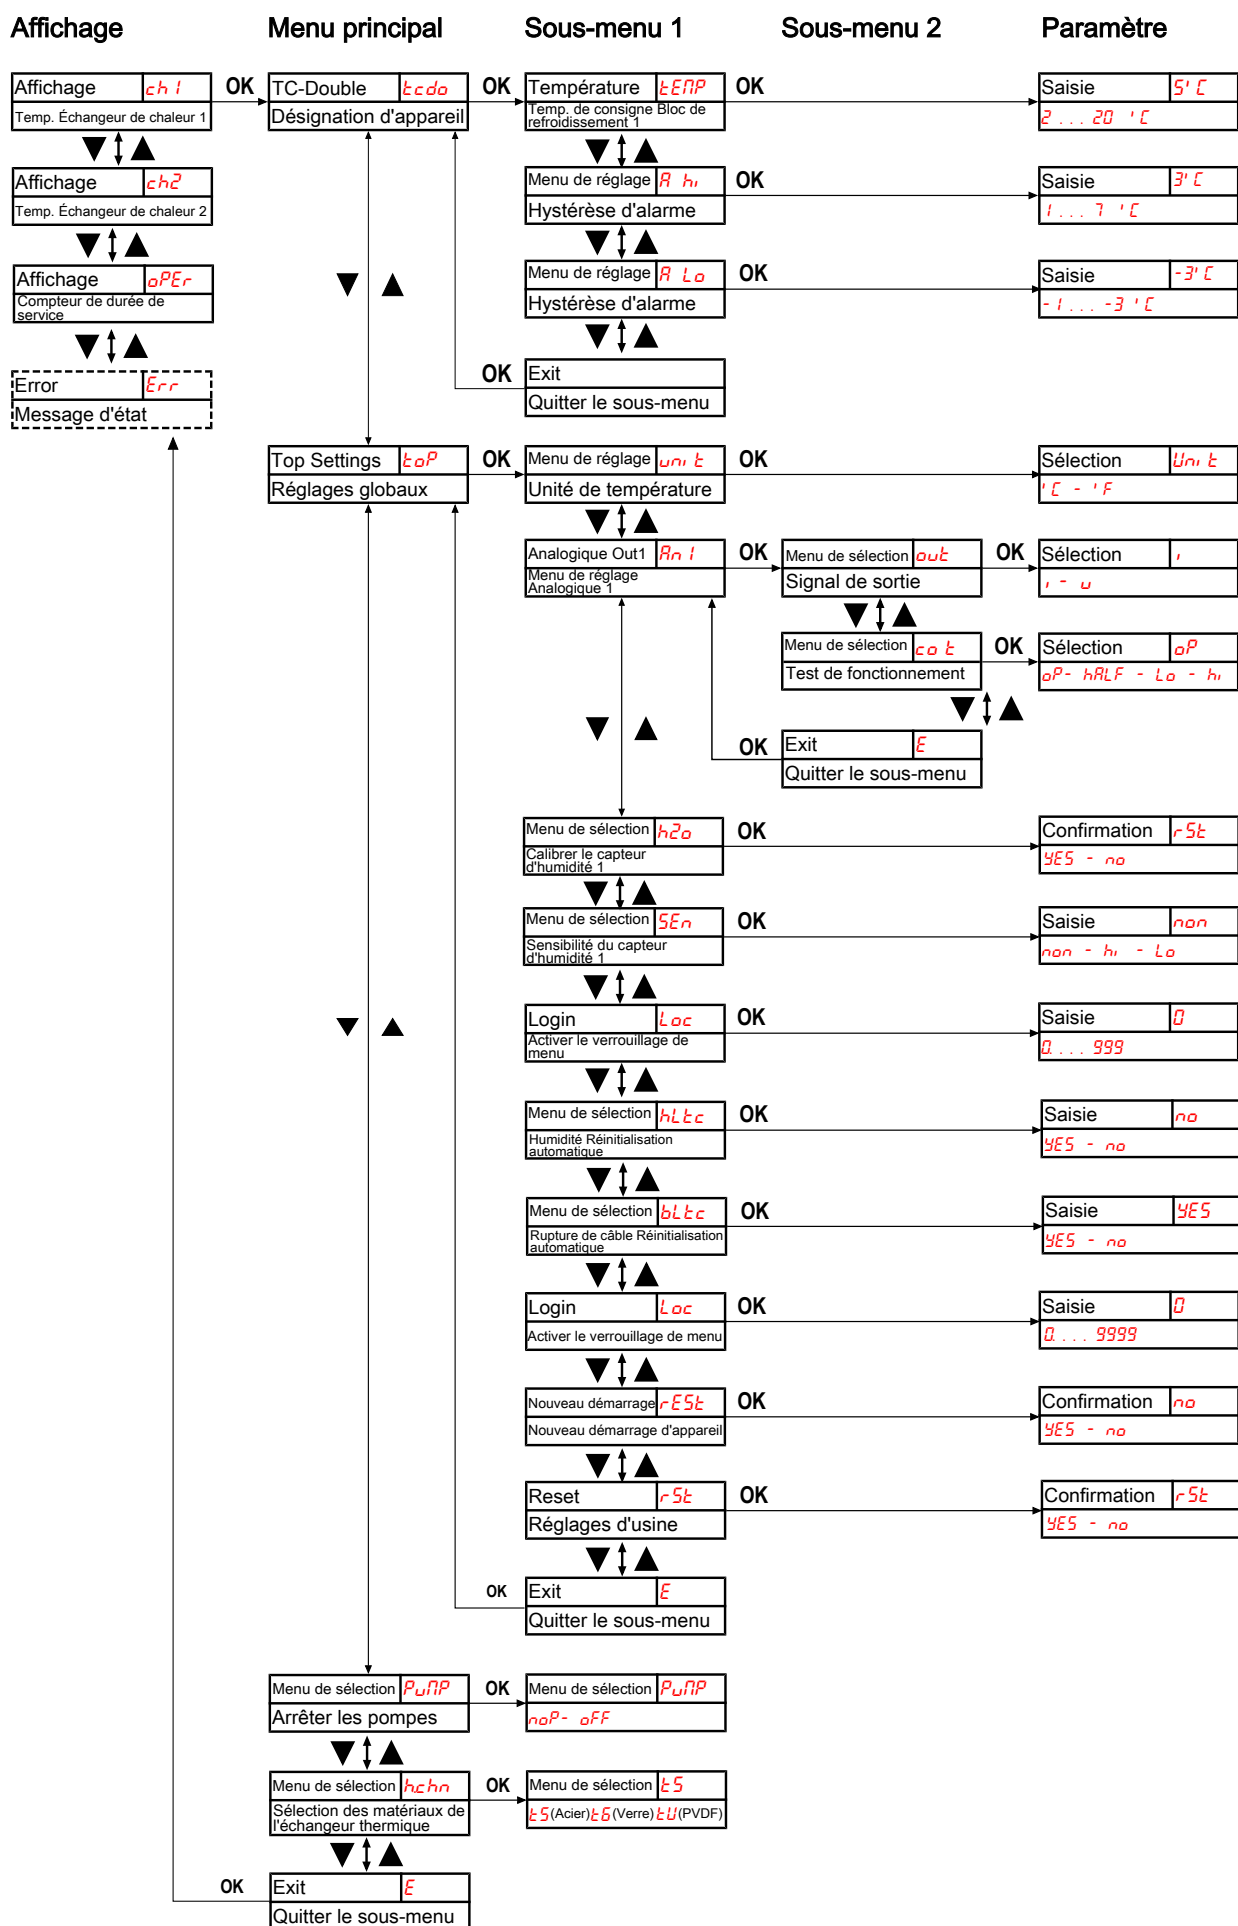



Fig. 1: Vue d'ensemble du menu TC-Double

5.3 Description des fonctions de menu

5.3.1 Menu d'affichage

Affichage de la température de bloc

Affichage → *ch1*



En fonction de l'état de l'appareil, la température est constante, clignotante ou affichée en alternance avec un message d'état.

Affichage des valeurs mesurées étape de pré-refroidissement

Affichage → *ch2*



En fonction de l'état de l'appareil, la température est constante, clignotante ou affichée en alternance avec un message d'état.

Affichage des heures de fonctionnement de l'appareil/de la durée de vie de l'appareil

Affichage → *oPEr*




Affichage des heures de fonctionnement de l'appareil. La durée de vie de l'appareil ne peut pas être réinitialisée et elle peut être exprimée dans différents formats d'affichage. Pour afficher/quitter l'affichage de l'heure d'exécution, appuyer sur la touche « Enter ».

- *yyMM* – Représentation en années et en mois (par défaut)
- *MMh* – Représentation en mois
- *WEEh* – Représentation en semaines
- *dDYS* – Représentation en jours
- Un mois correspond à une durée de 30 jours. Appuyer sur la touche « F » pour passer d'une forme de présentation à l'autre. Dans l'affichage, le format sélectionné est d'abord lisible sous forme de texte court, puis la durée.

Indication de code d'erreur

Affichage → *Err*



Si des défauts/défaillances hors service apparaissent, le numéro de défaut affiché indique les causes possibles et les mesures d'intervention.

5.3.2 Menu principal

Refroidisseur Peltier TC-Double

Visualisation → *tcdo*



On accède à partir d'ici au réglage de la température de consigne du refroidisseur et de la plage de tolérance (seuil d'alarme).

Réglage global


Affichage → *LoP* (ToP Settings)



Les réglages globaux pour le refroidisseur sont effectués dans ce menu.

Pompe péristaltique

Affichage → **PUMP**



Allumage et extinction de la pompe péristaltique.

Plage de paramètres : **noP, OFF**

Réglages d'usine : **noP**

Remarque : Le statut bascule, « **PUMP** » clignote.

Sélection des matériaux de l'échangeur thermique

Affichage → **hchh**



Sélection des matériaux de l'échangeur thermique

Plage de paramètres : **LS** (Acier), **LS** (Verre), **LU** (PVDF)

Réglages d'usine : **LS** (refroidisseur sans échangeur thermique), ou tout matériau selon la configuration

Exit menu principal

Affichage → **E**



Cette sélection permet de revenir au mode d'affichage.

5.3.3 Sous-menu 1

Température de consigne

Affichage → Refroidisseur → **LEMP**



Ce réglage fixe la valeur de consigne pour la température de refroidissement.

Plage de paramètres : de 2 °C à 20 °C (de 35,6 °F à 68 °F)


Réglages d'usine : 5 °C (41 °F)

Remarque : Lors d'une température modifiée, l'affichage clignote le cas échéant, jusqu'à ce que la nouvelle zone de travail soit atteinte.

Ce sous-menu n'est pas visible en cas de verrouillage de touche actif.

limite supérieure d'alarme

Affichage → Refroidisseur → **A hi** (Alarm high)



La valeur-seuil supérieure pour l'alarme optique et pour le relais d'alarme peut être réglée ici. Le seuil d'alarme est réglé en se basant sur la température de refroidissement déterminée.

Plage de paramètres : de 1 °C à 7 °C (de 1,8 °F à 12,6 °F)

Réglages d'usine : 3 °C (5,4 °F)

Remarque : Ce sous-menu n'est pas visible en cas de verrouillage de touche actif.

limite inférieure d'alarme

Affichage → Refroidisseur → **R Lo** (Alarm low)



La valeur-seuil supérieure pour l'alarme optique et pour le relais d'alarme peut être réglée ici. Le seuil d'alarme est réglé en se basant sur la température de refroidissement déterminée.

Plage de paramètres : de -1 °C à -3 °C (de -1,8 °F à -5,4 °F)

Réglages d'usine : -3 °C (-5,4 °F)

Remarque : Ce sous-menu n'est pas visible en cas de verrouillage de touche actif.

Exit sous-menu 1

Affichage → Sous-menu → **E**




En sélectionnant, on revient au menu principal.

5.3.4 Sous-menu 1 (réglages globaux)

Unité de température

Affichage → **LoP** → **Unit**




L'unité d'affichage de température peut être sélectionnée ici.

Plage de paramètres : 'C, 'F

Réglages d'usine : 'C

Sortie analogique

Affichage → **LoP** → **An 1**




Dans ce sous-menu sont définis les réglages de la sortie analogique 1, voir chapitre Sous-menu 2 (sortie analogique 1)

Remarque : Ce sous-menu n'est pas visible en cas de verrouillage de menu actif.

Étalonner le capteur d'humidité

Affichage → **LoP** → **h2o**



Lorsque les capteurs d'humidité sont installés, il est ici possible d'effectuer le calibrage. À cet effet, l'appareil doit être rincé au gaz sec.

Remarque : En usine, le calibrage a été effectué avec l'air ambiant. Il est nécessaire de renouveler le calibrage après avoir remplacé le capteur d'humidité.

Le calibrage du capteur d'humidité paramètre le menu **SEn** sur **hi**.

Ce sous-menu n'est pas visible en cas de verrouillage de menu actif.

Sensibilité Capteur d'humidité

Affichage → **LoP** → **SEn**



Lorsque les capteurs d'humidité sont installés, il est ici possible de réduire la sensibilité du capteur d'humidité.

Plage de paramètres : **hi** : sensibilité élevée
Lo : sensibilité faible
non : pas de capteur d'humidité

Réglages d'usine : **hi**

Remarque : Ce sous-menu n'est pas visible en cas de verrouillage de menu actif.

Capteur d'humidité : réinitialisation manuelle ou automatique après pénétration d'humidité

Affichage → **LoP** → **hLtc**

(**hLtc** = humidity latch). Le réglage vaut pour tous les capteurs d'humidité connectés.




Finalisation pour décider si le message pour pénétration d'humidité doit être réinitialisé manuellement ou bien réinitialisé automatiquement après séchage du capteur.

Plage de paramètres :	YES : L'état est signalé jusqu'au nouveau démarrage d'appareil par l'utilisateur, les pompes sont désactivées. no : Le message d'état est réinitialisé automatiquement/les pompes sont validées dès qu'aucune humidité n'est détectée.
Réglages d'usine :	no
Indication :	Ce sous-menu n'est pas visible en cas de verrouillage de menu actif.

Capteur d'humidité : réinitialisation automatique après rupture de câble

Affichage → **LoP** → **bLtc**

(**bLtc** = broken wire latch). Le réglage vaut pour tous les capteurs d'humidité connectés.




Finalisation pour décider si l'alarme pour rupture de câble doit être réinitialisée manuellement ou bien s'éteint d'elle-même en cas de signal de mesure valable.

Plage de paramètres :	YES : L'état est signalé jusqu'au nouveau démarrage d'appareil/l'acquittement de l'erreur par l'utilisateur, les pompes sont désactivées. no : Le message d'état s'éteint/les pompes sont de nouveau validées dès que le capteur d'humidité est de nouveau reconnu.
Réglages d'usine :	YES
Indication :	Ce sous-menu n'est pas visible en cas de verrouillage de menu actif.

Verrouillage de menu

Si vous souhaitez protéger le menu contre un accès non autorisé, saisissez ici une valeur pour le code de verrouillage. Certains points de menu sont ainsi accessibles seulement après la saisie du code correct.

Affichage → **LoP** → **LOc**



Ce réglage permet de désactiver voire d'activer le verrouillage de menu.

Plage de paramètres :	de 0 à 9999
Réglages d'usine :	0 (verrouillage de touches désactivé)
Indication :	Ce sous-menu n'est pas visible en cas de verrouillage de menu actif.

nouveau démarrage

Affichage → **LoP** → **rESt**

(**rESt** = restart)



L'appareil effectue un nouveau démarrage, tous les paramétrages sont conservés. Tous les messages d'erreur sont réinitialisés.

Le capteur d'humidité est réinitialisé indépendamment des réglages effectués dans les menus **hLtc** et **hLno**.

Plage de paramètres :	YES : Exécution du nouveau démarrage. L'écran indique les versions de logiciel de l'appareil et revient à l'affichage de valeur de mesure. no : Quitter le menu sans nouveau démarrage.
Indication :	Les paramétrages d'utilisateur sont conservés.

Réglages d'usine

Affichage → **LoP** → **r5t**



Ce réglage permet de rétablir les réglages d'usine.

Plage de paramètres : **YES** : rétablissement des réglages d'usine.

no : Quitter le menu sans modifications.

Réglages d'usine : **no**

Remarque : Ce sous-menu n'est pas visible en cas de verrouillage de menu actif.

Exit sous-menu 1

Affichage → Sous-menu → **E**



En sélectionnant, on revient au menu principal.

5.3.4.1 Sous-menu 2 (sortie analogique 1)

La température réelle du refroidisseur est indiquée à la sortie analogique.


Comportement de signal

En mode de fonctionnement normal (**noP**), la température réelle est indiquée à l'endroit de mesure. À des fins de test, les valeurs constantes **hi**, **Lo** ou **hRLF** peuvent être générées. Dans ce cas, un signal analogique est produit à la sortie analogique dont la valeur est indiquée dans le tableau.

Constante	Sortie de courant 4 – 20 mA	Sortie de tension 2 – 10 V
hi	20 mA	10 V
hi	12 mA	6 V
Lo	4 mA	2 V
noP	4 – 20 mA	2 – 10 V

Après le test, replacer impérativement le comportement de signal en fonctionnement normal (**noP**).

Anzeige → **LoP** → **Rn I** → **out**



Ce réglage permet de décider comment se comporte la sortie analogique.


Plage de paramètres : **noP** = Operation (fonctionnement normal), **hi**, **Lo**, **hRLF**

Réglages d'usine : **noP**

Indication : Ce sous-menu n'est pas visible en cas de verrouillage de menu actif.

Sélection -> Signal de sortie

Affichage → **LoP** → **Rn I** → **out**



Sélection du type de signal de sortie.

Plage de paramètres : **I** Sortie d'état 4... 20 mA

V Sortie d'état 2... 10 V

Réglages d'usine : **I**

Remarque : Débrancher l'appareil de mesure avant la reversion !

Ce sous-menu n'est pas visible en cas de verrouillage de touche actif.

Exit sous-menu 2

Affichage → *LoP* → *Rn I* → *E*



En sélectionnant, on revient au sous-menu 1.

5.3.5 Définir le menu favori

La touche **F** voire **Func** (touche de fonction) vous permet de définir un menu favori auquel vous pourrez accéder plus tard par une seule pression de touche.

- Affichez le menu que vous souhaitez définir comme favori. Le fait que ce menu puisse être ou non verrouillé n'a aucune d'importance.
- Pressez la touche de fonction pendant plus de 3 s.
Le menu actuel est défini comme favori. Le message *Func* apparaît brièvement sur l'afficheur.
- Revenez à l'affichage avec **ESC** ou *E* (Exit).

Si vous souhaitez maintenant afficher le menu favori, pressez le touche **F** voire **Func**.

INDICATION! Le menu favori est également accessible en cas de verrouillage de menu.

6 Entretien

Aucun travail de maintenance spécial n'est nécessaire sur le refroidisseur dans sa version de base.

Différentes options peuvent être incluses selon le type de refroidisseur. Dans ce cas-ci, les travaux de maintenance suivants doivent être effectués à intervalles réguliers :

- **Option Pompe péristaltique** : Vérification des tuyaux (voir chapitre Changer le tuyau de la pompe péristaltique (option))
- **Option filtre** : Vérification du l'élément du filtre (voir chapitre Changement de l'élément de filtre (option))
- **Option Capteur d'humidité** : Calibrage du capteur d'humidité (voir chapitre Calibrage du capteur d'humidité (option))
- **Option Pompe pour gaz de mesure** : Vérifier que les soupapes ne sont pas encrassées. Après 500 heures de fonctionnement, les vis de la bague de fixation sont à resserrer à 3 Nm. (voir chapitre Changement des valves d'admission et des soupapes d'échappement de la pompe pour gaz de mesure (en option))

Lors de toute opération de maintenance, respecter les points suivants :

- L'appareil ne doit être installé que par du personnel spécialisé et familiarisé avec les exigences de sécurité et les risques.
- Effectuez seulement les travaux de maintenance décrits dans ces instructions de commande et d'installation.
- Lorsque vous effectuez des travaux de maintenance de toute sorte, respectez les dispositions de sécurité et d'exploitation.
- N'utilisez que des pièces de rechange originales.

DANGER

Tension électrique

Danger d'électrocution



- a) Pour tous travaux, débranchez l'appareil du réseau.
- b) Assurez-vous que l'appareil ne puisse pas redémarrer involontairement.
- c) L'appareil ne peut être ouvert que par des personnels spécialisés qualifiés et instruits.
- d) Veillez à ce que l'alimentation électrique soit correcte.



DANGER

Gaz/condensats toxiques et irritants

Le gaz de mesure/les condensats peuvent être nocifs pour la santé.



- a) Le cas échéant, assurez une évacuation sûre du gaz/des condensats.
- b) Coupez l'arrivée de gaz lors de tous travaux d'entretien et de réparation.
- c) Lors des travaux d'entretien, protégez-vous des gaz/condensats toxiques/irritants. Portez l'équipement de protection approprié.



7 Entretien et réparation

Si une panne se produit en fonctionnement, vous trouverez dans ce chapitre des indications de détection et de résolution.

Les réparations sur les outils d'exploitation doivent être uniquement effectuées par le personnel autorisé par Bühler.

Si vous avez d'autres questions, veuillez vous adresser à notre service :

Tél. : +49-(0)2102-498955 ou votre représentant compétent

Vous trouverez de plus amples informations sur nos services de maintenance et de mise en service sous <https://www.buehler-technologies.com/service>.

Si le fonctionnement n'est pas correct après l'élimination d'éventuelles perturbations et après la mise sous tension, l'appareil doit être vérifié par le fabricant. À cet effet, veuillez expédier l'appareil dans un emballage approprié à :

Bühler Technologies GmbH

- Réparation/Maintenance -

Harkortstraße 29

40880 Ratingen

Allemagne

Ajoutez en outre à l'emballage la déclaration de décontamination RMA remplie et signée. Dans le cas contraire, il nous sera impossible de traiter votre demande de réparation.

Le formulaire se trouve en annexe à ce mode d'emploi. Il peut également être demandé par courriel :

service@buehler-technologies.com.

7.1 Recherche de panne et résolution



Problème / Défaillance	Cause possible	Assistance
Condensat dans la sortie de gaz	– Récipient collecteur de condensat plein	– Vider le récipient collecteur de condensat
	– Valve éventuellement bloquée dans le purgeur de condensat automatique	– Rincer dans deux directions
	– Refroidisseur surchargé	– Respecter les paramètres limites
Débit de gaz diminué	– Voies de gaz bouchées	– Démonter l'échangeur de chaleur et le nettoyer
	– Sortie de condensat gelée	– Remplacer l'élément de filtre le cas échéant
Température excessive	– Point de fonctionnement pas encore atteint	– Expédier l'appareil
	– Puissance de refroidissement trop faible, bien que le refroidisseur fonctionne	– Attendre (20 min. max.)
	– Débit / point de rosée / température de gaz trop élevé(e)	– Faire particulièrement attention à ne pas couvrir les fentes d'aération (accumulation de chaleur)
	– Ventilateur intégré à l'arrêt	– Respecter les paramètres limites / Prévoir un séparateur primaire
Sous-température	– Régulation défectueuse	– Vérifier et le remplacer le cas échéant
		– Expédier le refroidisseur


7.1.1 Messages d'erreur sur l'écran

Si une erreur apparaît, « *Err* » est affiché sur l'écran. Le(s) numéro(s) d'erreur est/sont affiché(s) en pressant la touche «  ».

Après détection de l'erreur, les messages d'erreur restent affichés tant que l'appareil n'est pas redémarré, ou que l'erreur soit acquittée en appuyant sur la touche « *Func* ». L'acquiescement fonctionne uniquement lorsque les circonstances de l'erreur ne sont plus présentes.

Causes / Assistance : Dans la liste suivante sont indiquées les causes et mesures les plus probables pour les erreurs respectives. Si les mesures indiquées ne devaient pas vous aider, veuillez vous adresser à notre service.

Problème/Défaillance		Cause possible	Assistance
Aucun affichage		– Aucune tension secteur – Conduite de raccordement desserrée – Écran défectueux	– Vérifier la conduite d'alimentation – Vérifier le fusible – Vérifier les raccordements
 D1.02 (en continu)		(La version logicielle de l'écran est affichée). – Pas de communication vers le régulateur	– Vérifier les raccordements
 Error		– Une erreur est détectée	– Lecture du numéro d'erreur comme décrit ci-dessus
 Error 01		– Défaillance de régulateur	– Acquitter l'erreur (dysfonctionnement temporaire) – Couper la tension d'alimentation électrique durant env. 5 s – Informer le service
		– Défaillance du régulateur 2	– Acquitter l'erreur (dysfonctionnement temporaire) – Couper la tension d'alimentation électrique durant env. 5 s – Informer le service
 Error 03		– Défaillance de microcontrôleur/MCP2	– Informer le service
 Error 04		– Erreur EEPROM	– Informer le service
		– Défaut du ventilateur/ventilateur hors service	– Vérifier ventilateur (bloqué ?) – Vérifier raccordement
 Error 22		– Rupture de câble Capteur d'humidité 1	– Contrôler la conduite du capteur d'humidité – Contrôler le capteur d'humidité
 Error 32		– Rupture de câble Capteur d'humidité 2	– Contrôler la conduite du capteur d'humidité – Contrôler le capteur d'humidité
 Error 40		– Erreur générale Capteur de température 1 (température de bloc)	– Capteur possiblement défectueux
 Error 41		– Sous-température/Court-circuit Capteur de température 1	– Vérifier le raccordement du capteur de température
 Error 42		– Sur-température/Court-circuit Capteur de température 1	– Vérifier le raccordement du capteur de température
 Error 43		– Fluctuation de la valeur mesurée Capteur de température 1	– Vérifier le raccordement du capteur de température
 Error 50		– Erreur générale Capteur de température 2 (température de bloc)	– Capteur possiblement défectueux
 Error 51		– Sous-température/Court-circuit Capteur de température 2	– Vérifier le raccordement du capteur de température
 Error 52		– Sur-température/Court-circuit Capteur de température 2	– Vérifier le raccordement du capteur de température
 Error 53		– Fluctuation de la valeur mesurée Capteur de température 2	– Vérifier le raccordement du capteur de température

Texte d'état	Cause possible	Assistance
 H2o.1	– Alarme d'humidité Capteur d'humidité 1	– Sécher – Vérifier le récipient collecteur de condensat
 init	– Phase d'initialisation	– Attendre
 PuMP	– Pompes désactivées	– Réactiver les pompes dans le menu
 dt	Uniquement lors d'une régulation active du Delta T : La température du bloc ne se trouve pas dans la plage de température définie. – Le refroidisseur se trouve encore en « phase de démarrage ». – Température ambiante variable – Puissance de refroidissement non suffisante	– Attendre de voir si la température cible est atteinte – Contrôler la température ambiante /la puissance obtenue – Selon le processus : adapter les seuils d'alarme
 (clignotement)	– Sur-/Sous-température	– voir chapitre « Recherche de cause de panne et résolution »

7.2 Indications de sécurité

- L'appareil ne doit pas être utilisé dans un cadre extérieur à ses spécifications.
- Les réparations sur le matériel doivent être effectuées uniquement par des personnels autorisés de Bühler.
- Effectuez des travaux de modification, de montage ou d'entretien uniquement si ceux-ci sont décrits dans les instructions d'utilisation et d'installation.
- Utilisez uniquement des pièces de rechange d'origine.

DANGER

Tension électrique

Danger d'électrocution



- Pour tous travaux, débranchez l'appareil du réseau.
- Assurez-vous que l'appareil ne puisse pas redémarrer involontairement.
- L'appareil ne peut être ouvert que par des personnels spécialisés qualifiés et instruits.
- Veillez à ce que l'alimentation électrique soit correcte.



DANGER

Gaz/condensats toxiques et irritants

Le gaz de mesure/les condensats peuvent être nocifs pour la santé.



- Le cas échéant, assurez une évacuation sûre du gaz/des condensats.
- Coupez l'arrivée de gaz lors de tous travaux d'entretien et de réparation.
- Lors des travaux d'entretien, protégez-vous des gaz/condensats toxiques/irritants. Portez l'équipement de protection approprié.



ATTENTION

Risque pour la santé en cas de non-étanchéité de l'échangeur de chaleur

L'échangeur de chaleur est rempli d'un agent de refroidissement à base de glycol.

En cas de non-étanchéité de l'échangeur de chaleur :



- évitiez tout contact avec la peau et les yeux.
- En cas de fuite de l'échangeur de chaleur, ne remettez pas le refroidisseur en marche. Le refroidisseur doit être réparé par le fabricant.

7.3 Nettoyage et démontage de l'échangeur de chaleur

Les échangeurs thermiques ne doivent être remplacés ou entretenus que s'ils sont bouchés ou abîmés. Dans le cas où ils se bouchent, nous recommandons de vérifier si ce problème peut être évité à l'avenir en utilisant un filtre.

- Couper l'alimentation de gaz.
- Éteindre l'appareil et débrancher toutes les fiches (p. ex. fiche de raccordement d'analyseur de sortie d'état, entrée d'alimentation etc.).
- Débrancher les raccords de gaz et l'écoulement du condensat.
- Tirer l'échangeur thermique vers le haut.
- Nettoyer le nid de refroidissement (trou dans le bloc de refroidissement), étant donné que les échangeurs thermiques sont utilisés avec de la graisse siliconée.
- Rincer l'échangeur thermique jusqu'à élimination complète des impuretés.
- Lubrifier l'échangeur thermique sur la surface extérieure refroidie à l'aide de graisse siliconée.
- Introduire de nouveau l'échangeur dans le nid de refroidissement en effectuant un mouvement de rotation.
- Rétablir les raccords de gaz et l'écoulement du condensat. L'entrée de gaz est marquée en rouge.
- Rétablir l'alimentation en tension/l'admission de gaz et attendre la disponibilité à fonctionner.
- Ouvrir l'admission de gaz.

7.4 Changer le tuyau de la pompe péristaltique (option)

- Couper l'admission de gaz.
- Éteindre l'appareil et débrancher toutes les fiches (p. ex. fiche de raccordement d'analyseur de sortie d'état, entrée d'alimentation etc.).
- Retirer le tuyau d'alimentation et d'évacuation sur la pompe péristaltique (**Observer les indications de sécurité !**).
- Desserrer la vis à tête moletée centrale sans la dévisser entièrement. Basculer la vis vers le bas.
- Retirer le couvercle vers le haut.
- Extraire les raccords sur les côtés et retirer le tuyau.
- Remplacer le tuyau (pièce de rechange Bühler) et monter la pompe péristaltique dans l'ordre inverse.
- Rétablir l'alimentation en tension ainsi qu'en gaz.

7.5 Changement de l'élément de filtre (option)

ATTENTION



Émanations de gaz du filtre

Le filtre ne doit pas être sous pression lorsqu'il est démonté.
Ne réutilisez pas les pièces ou joints toriques endommagés.

- Couper l'alimentation de gaz.
- Mettre l'appareil hors tension et débrancher la fiche d'alimentation.
- Tirer la bride tout en maintenant le verre de filtre.
- Tout en maintenant la tête de filtre et en effectuant de légers mouvements de va-et-vient, retirer le verre vers le bas.
- Retirer l'élément de filtre usagé puis en placer un nouveau.
- Vérifier le joint, le remplacer le cas échéant.
- Tout en maintenant la tête de filtre et en effectuant de légers mouvements de va-et-vient, emboîter la bride et veiller à une bonne assise.
- Rétablir l'alimentation en tension ainsi que l'admission de gaz.

INDICATION! Les réglementations légales pour la mise au rebut d'éléments de filtre doivent être respectées.


7.6 Séchage du capteur d'humidité (option)

Après une infiltration d'humidité, le capteur d'humidité doit être séché.

- Couper l'alimentation de gaz.
- Mettre l'appareil hors tension et débrancher la fiche d'alimentation.
- Desserrer l'écrou d'accouplement de la ligne de raccordement du capteur d'humidité et extraire la ligne.
- Tourner le capteur d'humidité dans le sens inverse des aiguilles d'une montre et l'extraire.
- Sécher le capteur d'humidité.
- Replacer le capteur d'humidité et serrer le vissage avec précautions.
- Emboîter la ligne de raccordement et serrer l'écrou d'accouplement.
- Rétablir l'alimentation en tension ainsi que l'admission de gaz.

7.7 Calibrage du capteur d'humidité (option)

- Lorsque les capteurs d'humidité ont été remplacés, il doivent être recalibrés.
- S'assurer que le gaz sec a été dirigé par le refroidisseur.
- Sélectionner et confirmer le menu du refroidisseur.



- Sélectionner le point du menu du capteur d'humidité.



- L'écran indique (Reset).
- En confirmant l'écran, le capteur d'humidité est calibré.

Un aperçu exact du guidage par menu se trouve dans le chapitre « Fonctionnement et maniement ».

7.8 Changement des valves d'admission et des soupapes d'échappement de la pompe pour gaz de mesure (en option)



Démontez tout d'abord les raccords à visser.


Extrayez la valve d'admission voire d'évacuation en la tournant au moyen d'un tournevis large et plat.

Attention : Dans le cas des corps de pompe PVDF et PVDF avec soupape by-pass, des bagues d'étanchéité PTFE sont intégrées dans les entrées et sorties de gaz. Elles sont également jointes à votre kit de pièces de rechange pour soupape. Retirez les bagues d'étanchéité usagées avant de mettre les neuves en place.

Les valves d'admission et d'évacuation sont identiques. Leur position de montage détermine leur fonctionnalité. Comme indiqué sur la figure, les valves sont bleues d'un côté et noires de l'autre. De plus, les valves sont caractérisées par « EIN » voire « IN » pour Admission et « AUS » voire « OUT » pour Évacuation.

Soupape d'admission

Soupape d'échappement

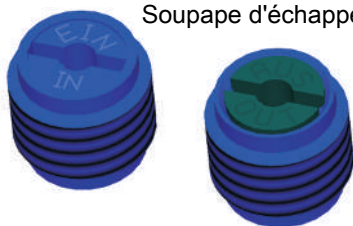


Concernant l'assemblage de la pompe pour gaz de mesure, effectuez les étapes dans l'ordre inverse. Lors du serrage des valves d'admission et d'évacuation, respectez impérativement le couple de vissage prescrit maximal de 1 Nm. **ATTENTION! Un serrage plus important des valves conduit à une déformation durable du corps de pompe, ce qui nécessiterait un remplacement.**



Lors de la mise en place des raccords à visser, veillez à l'étanchéité du raccord.

7.9 Remplacement du joint torique de soupape by-pass (en option)

- Desserrer les deux vis sur la plaque de soupape et extraire avec précaution la totalité de l'unité.
- Humidifier le nouveau joint torique avec une graisse pour joint torique appropriée (température d'utilisation continue minimum 145 °C, par exemple Fluoronox S90/2) et l'appliquer sur la broche.
- Introduire avec précaution la totalité de l'unité dans le carter de pompe et serrer les vis.

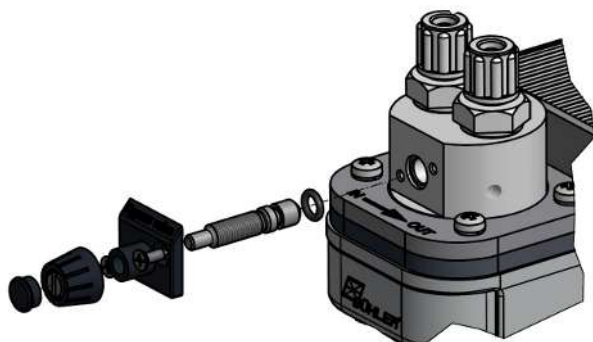

7.10 Changement du joint à soufflet (en option)

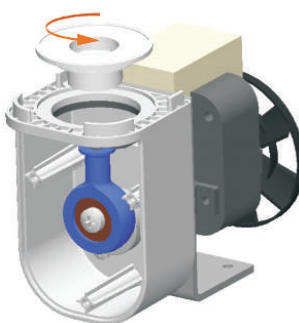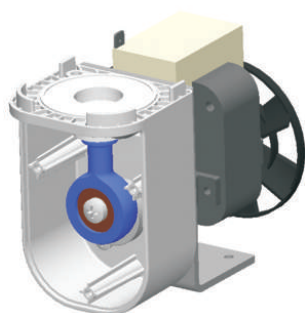

Pour changer le soufflet, dévissez-le avec précaution du coulisseau en le tournant dans le sens inverse des aiguilles d'une montre. Faites attention à ne pas perdre les éventuelles rondelles d'ajustement.

Avant de remettre en place le soufflet, faites attention à ce que celui-ci ne présente aucun dégât.

Le montage se fait à la main en suivant les étapes en sens inverse.

7.11 Pièces de rechange

Lors de la commande de pièces de rechange, nous vous demandons d'indiquer le type d'appareil et le numéro de série.

Vous pouvez trouver des ensembles de rééquipement et des ensembles supplémentaires dans notre catalogue.

Vous devriez avoir une réserve des pièces de rechanges suivantes :

N° d'article	Désignation
9100100007	Module d'affichage MCD400
9144050080	Câble de raccordement Module d'affichage de platine de régulateur, 400 mm
9144050091	Câble de raccordement Mainboards
9100130380	Platine de microcontrôleur MCP2.2
9100132380	Platine de microcontrôleur MCP2.2 ADON
4011000	Adaptateur de débit de type G, PVDF G1/4
40110001	Adaptateur de débit de type NPT, PVDF NPT 1/4"
4011005	Adaptateur de débit de type G, acier inoxydable, G1/4
40110051	Adaptateur de débit de type NPT, acier inoxydable, NPT 1/4"
4111100	Capteur d'humidité FF-3-N, sans câble
9144050081	Câble de raccordement du capteur d'humidité, 300 mm
9144050082	Capteur d'humidité Câble de raccordement, 450 mm
449600062	Ventilateur, 12 V DC avec sortie d'état
9100010198	Circuit imprimé de réseau
9100011187	Module de contrôle
voir fiche technique 450022	Pompes péristaltiques CPsingle, CPdouble X2
voir fiche technique 450013	Pompes de circulation P1.3

7.11.1 Consommables et accessoires


N° d'article	Désignation
4510008	Dérivateur de condensat automatique AK 5.2 (uniquement fonctionnement sous pression)
4510028	Dérivateur de condensat automatique AK 5.5 (uniquement fonctionnement sous pression)
4410004	Dérivateur de condensat automatique AK 20 (uniquement fonctionnement sous pression)
4410001	Dérivateur de condensat automatique 11 LD V 38 (uniquement fonctionnement sous pression)
41030050	Élément de rechange de filtre F2 ; VE 5 pièces
9144050038	Câble pour sortie analogique Température de refroidisseur 4 m
4410005	Récipient collecteur de condensat GL1, 0,4 l
44920035012	Tuyau de rechange pompe à condensat, Tygon (Norprene), raccord de tuyau coudé
44920035016	Tuyau de rechange pompe à condensat, Tygon (Norprene), raccord de tuyau coudé et vis (métriques)
44920035017	Tuyau de rechange pompe à condensat, Tygon (Norprene), raccord de tuyau coudé et vis (en pouces)
4228003	Joint à soufflet pour pompe P1
9009398	Joint torique pour pompe by-pass P1
4228066	Jeu de soupape d'entrée/de sortie 70 °C pour pompe P1

8 Mise au rebut

L'échangeur de chaleur contient un liquide de refroidissement à base de glycol.

Lors de la mise au rebut des produits, les prescriptions légales nationales respectivement applicables doivent être prises en compte et respectées. Aucun risque pour la santé et l'environnement ne doit résulter de la mise au rebut.

Le symbole de poubelle barrée sur roues apposé sur les produits de Bühler Technologies GmbH signale des consignes de mise au rebut particulières au sein de l'Union Européenne (UE) applicables aux produits électriques et électroniques.



Le symbole de poubelle barrée signale que les produits électriques et électroniques ainsi désignés ne doivent pas être jetés avec les ordures ménagères. Ils doivent être éliminés de manière appropriée comme appareils électriques et électroniques.

Bühler Technologies GmbH s'occupe volontiers de la mise au rebut de votre appareil arborant ce sigle. Veuillez pour ceci envoyer votre appareil à l'adresse ci-dessous.



La loi nous oblige à protéger nos employés des risques causés par des appareils contaminés. Nous ne pouvons donc effectuer la mise au rebut de votre ancien appareil que si celui-ci ne contient pas d'agents de fonctionnement agressifs, corrosifs ou nocifs pour la santé et l'environnement. Nous vous prions donc de faire preuve de compréhension. **Pour chaque appareil électrique et électronique usagé, il convient d'établir le formulaire « Formulaire RMA et déclaration de décontamination » disponible sur notre site Internet. Le formulaire rempli doit être apposé sur l'emballage de manière visible de l'extérieur.**

Pour le retour d'appareils électriques et électroniques usagés, veuillez utiliser l'adresse suivante :

Bühler Technologies GmbH
WEEE
Harkortstr. 29
40880 Ratingen
Allemagne

Tenez compte des règles en matière de protection de données et du fait que vous êtes responsable de l'absence de toute donnée personnelle sur les anciens appareils rapportés par vos soins. Assurez-vous donc de bien supprimer toute donnée personnelle lors de la restitution de votre appareil usagé.

9 Pièces jointes

9.1 Données techniques refroidisseur à gaz

Caractéristiques techniques du refroidisseur à gaz

Disponibilité à fonctionner	après 10 minutes max.			
Température ambiante	de 5 °C à 60 °C			
Point de rosée de sortie de gaz préréglé : réglable :	5 °C 2 °C...20 °C			
Type de protection	IP 20			
Boîtier	Acier inoxydable, brossé			
Dimensions d'emballage	env. 427 x 300 x 293 mm			
Poids incl. échangeur thermique	env. 11,5 kg env. 15 kg pour une phase de développement complète			
Données électriques	Appareil sans extension		Appareil avec extension (pompe péristaltique + pompe à gaz)	
	230 V AC	115 V AC	230 V AC	115 V AC
	+5/-10 %	+5/-10 %	+5 %	+5 %
	50/60 Hz	50/60 Hz	50 Hz	60 Hz
	1,6 A	3,2 A	2,1 A	4,1 A
	278 W / 350 VA	296 W / 370 VA	390 W / 487 VA	377 W / 472 VA
Fusible recommandé (caractéristique : lent)	2,5 A	4 A	2,5 A	5 A
Puissance de commutation sortie d'état	max. 250 V AC, 150 V DC 2 A, 50 VA, hors tension			
Raccordements électriques	Fiche selon EN 175301-803			
Raccordements de gaz	Échangeur thermique voir tableau « Vue d'ensemble des échangeurs thermiques » Filtre, adaptateur de capteur d'humidité, pompe à gaz, G1/4 ou NPT 1/4" voire tuyau ou tube métrique/pouces			
Éléments en contact avec les fluides Filtre : Capteur d'humidité : Échangeur thermique : Pompe péristaltique : Tubulure :	voir « Données techniques Options » voir « Données techniques Options » voir tableau « Vue d'ensemble des échangeurs thermiques » voir « Données techniques Options » PTFE/Viton			
Marquages :	FM18ATEX0012X : II 3 G Ex ec nC IIC T4 Gc IECEX FMG 18.0005X : Ex ec nC IIC T4 Gc FM18US0021X/FM18CA0010X : CL I DIV 2 GP ABCD RU C-DE.HA65.B.00608/20			

9.2 Caractéristiques techniques options

Données techniques Sortie analogique Température du refroidisseur

Signal	4-20 mA voire 2-10 correspond à une température de refroidisseur de -20 °C à +60 °C
Raccordement	Ficher M12x1, DIN EN 61076-2-101

Données techniques Capteur d'humidité FF-3-N

Température ambiante	de 3 °C à 50 °C
pression de service max. avec FF-3-N	2 bar
Matériau	PVDF, PTFE, résine époxy, acier inoxydable 1.4571, 1.4576

Données techniques pompe péristaltique CPdouble X2

Température ambiante	de 0 °C à 50 °C
Puissance de débit	0,3 l/h (50 Hz) / 0,36 l/h (60 Hz) avec tuyau standard
Entrée de vide	max. 0,8 bar
Pression d'entrée	max. 1 bar
Pression de sortie	1 bar
Tuyau	4 x 1,6 mm
Type de protection	IP 44
Matériaux	
Tuyau :	Norprene (standard), Marprene, Fluran
Raccordements :	PVDF


Données techniques pompe pour gaz de mesure P1.3

Température ambiante	de 0 °C à 50 °C
Pression de fonctionnement	max. 1,3 bar abs.
Débit de convoyage nominal	280 l/h (pour p = 1 bar abs.)
Matériaux en contact avec le fluide selon la configuration	PTFE, PVDF, 1.4571, 1.4401, Viton

Données techniques Filtre AGF-PV-30-F2

Température ambiante	de 3 °C à 100 °C
pression de service max. avec filtre	4 bar
Surface de filtre	60 cm ²
Finesse de filtre	2 µm
Volume mort	57 ml
Matériau :	
Filtre :	PVDF, verre Duran (pièces en contact avec les fluides)
Joint :	Viton
Élément de filtre :	PTFE fritté

9.3 Schéma de procédé

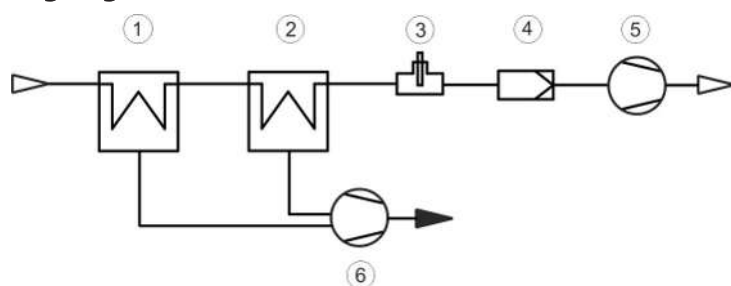
Organigramme :

1 Échangeur de chaleur 2 /refroidissement préalable	4 Filtre (en option)
2 Échangeur de chaleur 1 /refroidissement subséquent	5 Pompe pour gaz de mesure (en option)
3 Capteur d'humidité (en option)	6 Pompe de condensat (en option)


9.4 Courbes de puissance

Le TC-Double 6111 (X2) est conçu pour une température ambiante allant jusqu'à 40 °C. Une puissance de refroidissement suffisante est disponible avant d'atteindre cette température. Au contraire, le TC-Double 6112 (X2) est utilisable pour des températures plus élevées jusqu'à une température nominale de 60 °C. Veuillez respecter la puissance de refroidissement existante.

Type TC-Double 6111 (X2)

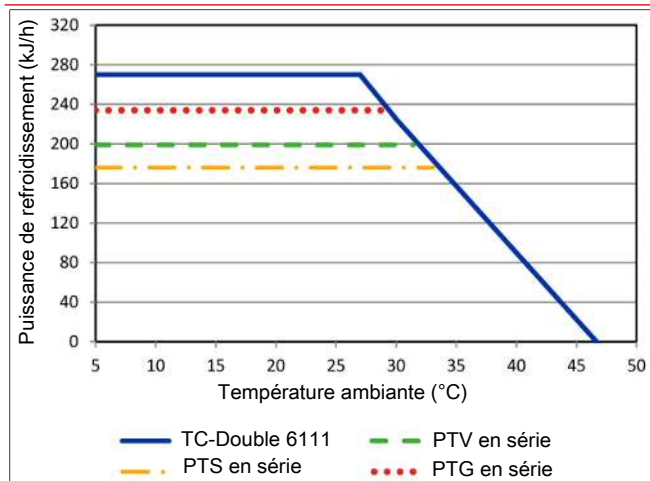


Type TC-Double 6112 (X2)

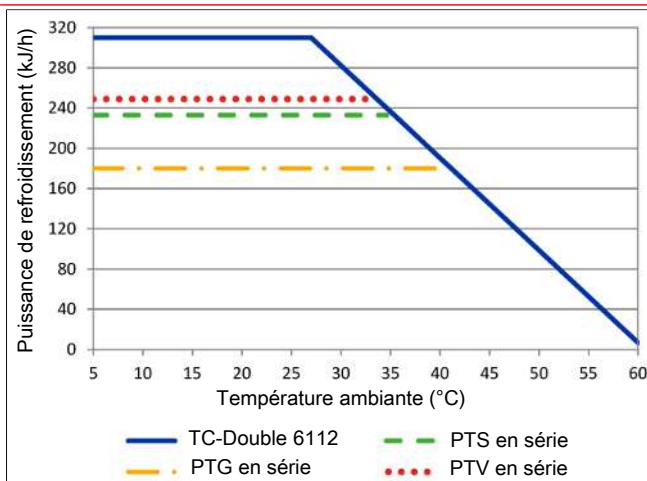


Remarque : Les courbes limites pour les échangeurs thermiques s'appliquent pour un point de rosée de 50 °C.

Le TC-Double 6111 (X2) est conçu pour une température ambiante allant jusqu'à 40 °C. Une puissance de refroidissement suffisante est disponible avant d'atteindre cette température. Au contraire, le TC-Double 6112 (X2) est utilisable pour des températures plus élevées jusqu'à une température nominale de 60 °C. Veuillez respecter la puissance de refroidissement existante.

Type TC-Double+ 6111 (X2)

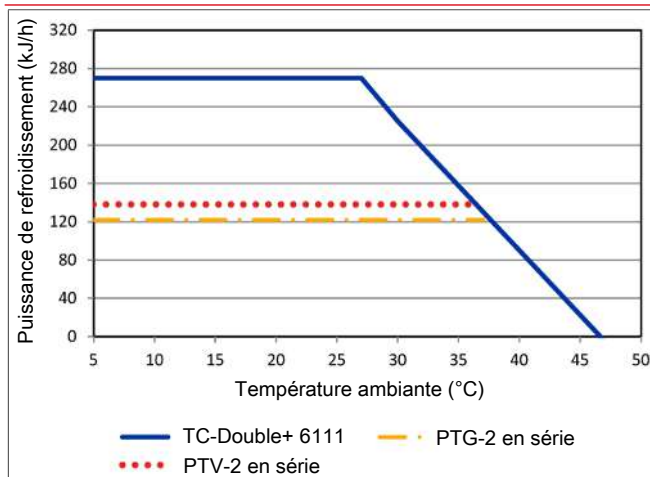

Type TC-Double+ 6112 (X2)

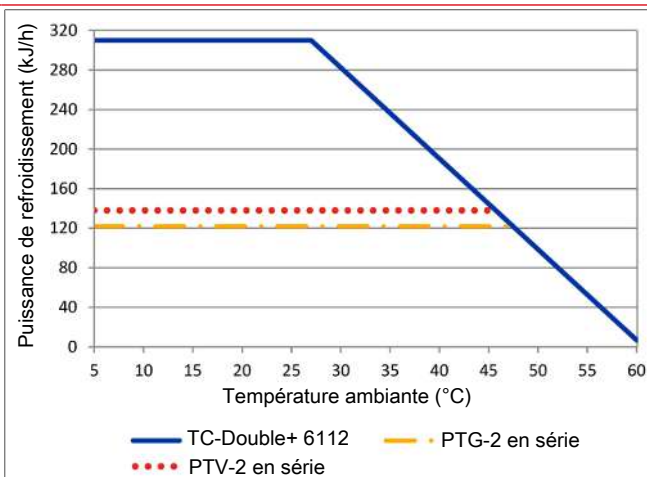

Remarque : Les courbes limites pour les échangeurs thermiques s'appliquent pour un point de rosée de 50 °C.

9.5 Échangeur thermique

9.5.1 Description échangeur de chaleur

L'énergie du gaz de mesure et en première approche la performance de refroidissement sollicitée Q est déterminée par les trois paramètres température de gaz ϑ_g , point de rosée r_e (taux d'humidité) et débit v . Pour des raisons physiques, le point de rosée de sortie augmente avec l'énergie de gaz. Les limites suivantes pour le débit maximal sont déterminées pour un point de travail normé de $r_e = 50$ °C et $\vartheta_g = 70$ °C. Le débit maximal $v_{\max}$ est indiqué en m^3/h d'air refroidi, c'est-à-dire après la condensation de la vapeur d'eau. Les valeurs peuvent diverger pour les autres points de rosée et températures d'entrée de gaz. Les liens physiques sont cependant si nombreux qu'une représentation sera exclue. Si certains points ne sont pas clairs, veuillez nous consulter ou utiliser notre programme d'organisation.

9.5.2 Vue d'ensemble de l'échangeur thermique

TC-Double

Échangeur de chaleur	2x PTS 2x PTS-I ²⁾	2x PTG 2x PTG-I ²⁾	2x PTV 2x PTV-I ²⁾
Matériaux en contact avec les fluides	Acier inoxydable	Verre PTFE	PVDF
Débit $v_{\max}$ ¹⁾	450 l/h	250 l/h	250 l/h
Point de rosée d'entrée $\tau_{e,\max}$ ¹⁾	70 °C	70 °C	70 °C
Température d'entrée de gaz $\vartheta_{G,\max}$ ¹⁾	180 °C	140 °C	140 °C
Max. Puissance de refroidissement $Q_{\max}$	310 kJ/h	215 kJ/h	295 kJ/h
Pression de gaz $p_{\max}$	3 bar ⁴⁾	3 bar	2 bar
Pression différentielle Δp ($v=150$ l/h) au total	20 mbar	20 mbar	20 mbar
Volumes morts V_{mort} au total	59 ml	59 ml	115 ml
Raccordements gaz (métrique)	6 mm	GL 14 (6 mm) ³⁾	DN 4/6
Raccordements gaz (en pouces)	1/4"	GL 14 (1/4") ³⁾	1/4"-1/6"
Purgeur de condensat (métrique)	G3/8	GL 25 (12 mm) ³⁾	G3/8
Purgeur de condensat (en pouces)	NPT 3/8"	GL 25 (1/2") ³⁾	NPT 3/8"

¹⁾ Tenant compte de la puissance maximale de refroidissement du refroidisseur.

²⁾ Les types comprenant un I sont pourvus de filetages NPT, voire de tubes en pouces.

³⁾ Diamètre intérieur de la bague d'étanchéité.

⁴⁾ 160 bar sur demande.

TC-Double+


Échangeur de chaleur	2x PTG-2 2x PTG-2-I ²⁾	2x PTV-2 2x PTV-2-I ²⁾
Matériaux en contact avec les fluides	Verre PTFE	PVDF
Débit $v_{\max}$ ¹⁾	250 l/h	250 l/h
Point de rosée d'entrée $\tau_{e,\max}$ ¹⁾	70 °C	70 °C
Température d'entrée de gaz $\vartheta_{G,\max}$ ¹⁾	140 °C	140 °C
Max. Puissance de refroidissement $Q_{\max}$	230 kJ/h	215 kJ/h
Pression de gaz $p_{\max}$	3 bar	2 bar
Pression différentielle Δp ($v=150$ l/h) au total	20 mbar	20 mbar
Volumes morts V_{mort} au total	59 ml	115 ml
Raccordements gaz (métrique)	GL 14 (6 mm) ³⁾	DN 4/6
Raccordements gaz (en pouces)	GL 14 (1/4") ³⁾	1/4"-1/6"
Purgeur de condensat (métrique)	GL 25 (12 mm) ³⁾	G3/8
Purgeur de condensat (en pouces)	GL 25 (1/2") ³⁾	NPT 3/8"

¹⁾ Tenant compte de la puissance maximale de refroidissement du refroidisseur.

²⁾ Les types comprenant un I sont pourvus de filetages NPT, voire de tubes en pouces.

³⁾ Diamètre intérieur de la bague d'étanchéité.

9.6 Dimensions (mm)

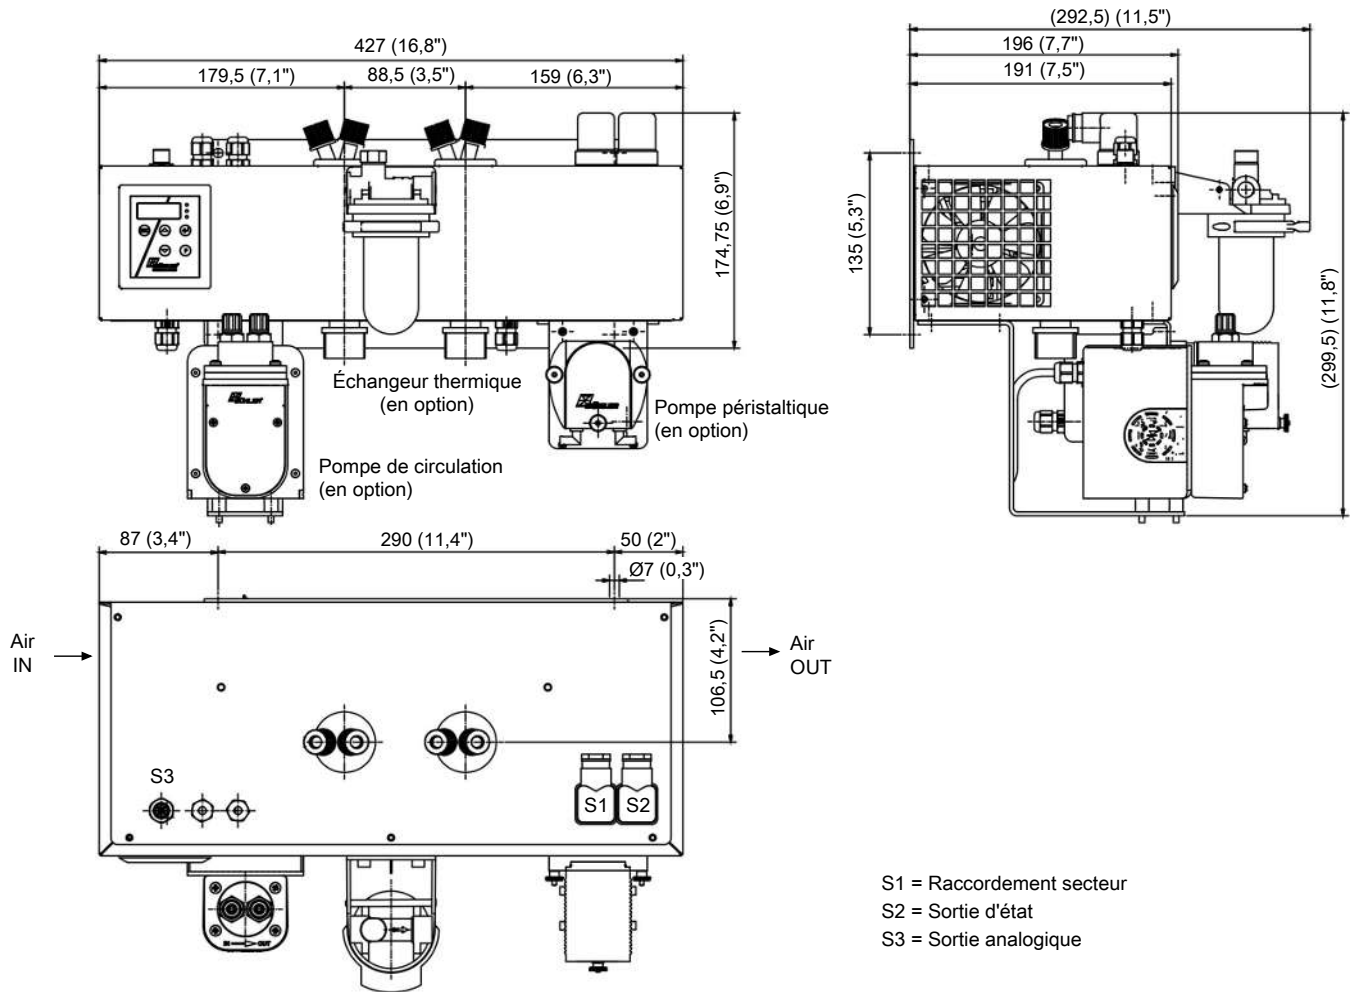

10 Documents joints

- Déclaration de conformité
- Certificats
- RMA - Déclaration de décontamination

EU-Konformitätserklärung EU-declaration of conformity



Hiermit erklärt Bühler Technologies GmbH, dass die nachfolgenden Produkte den wesentlichen Anforderungen der Richtlinie

Herewith declares Bühler Technologies GmbH that the following products correspond to the essential requirements of Directive

2014/34/EU
(Atex)

in ihrer aktuellen Fassung entsprechen.

in its actual version.

Produkt / products: Messgaskühler / Sample gas cooler
Typ / type: TC-Standard X2, TC-MIDI X2, TC-Double X2
TC-Standard+ X2, TC-MIDI+ X2, TC-Double+ X2

Die Produkte werden entsprechend der derzeit gültigen Atex-Richtlinie innerhalb der internen Fertigungskontrolle folgendermaßen gekennzeichnet:

The products are marked according to the currently valid Atex directive during internal control of production:

Atex:  II 3 G Ex ec nC IIC T4 Gc
IECEx: Ex ec nC IIC T4 Gc

Die Eignung dieses Produkts für die Zone 2 wurde durch eine Baumusterprüfbescheinigung mit der Nummer FM18ATEX0012X festgestellt.

Die Betriebsanleitung zu diesem Produkt beinhaltet besondere Installations- und Betriebsbedingungen und sind für die sichere Anwendung zu beachten.

This product's suitability for Zone 2 was determined by type-examination certificate number FM18ATEX0012X.

The operating instructions for this product contains special installation and operating conditions and must be observed to ensure safe operation.

Zur Beurteilung der Konformität wurden folgende harmonisierte Normen herangezogen:
For the assessment of conformity the following standards have been used:

EN 60079-0:2012 + A11:2013

EN 60079-7:2015+A1:2018

EN 60079-15:2018

Der Hersteller hat die Übereinstimmung des Gerätes mit aktuelleren Normenausgaben als in der Baumusterprüfbescheinigung aufgeführt geprüft und die Konformität festgestellt:

The manufacturer has checked the compliance of the device with more current standards than those listed in the type examination certificate and has established conformity:


EN IEC 60079-0:2018

EN IEC 60079-7:2015 + A1:2018

Dokumentationsverantwortlicher für diese Konformitätserklärung ist Herr Stefan Eschweiler mit Anschrift am Firmensitz.

The person authorised to compile the technical file is Mr. Stefan Eschweiler located at the company's address.

Ratingen, den 01.03.2021


Stefan Eschweiler
Geschäftsführer – Managing Director


Frank Pospiech
Geschäftsführer – Managing Director

CERTIFICATE OF CONFORMITY



1. **HAZARDOUS LOCATION ELECTRICAL EQUIPMENT PER CANADIAN REQUIREMENTS**
2. **Certificate No:** FM18CA0010X
3. **Equipment:** TC-Standard X2; TC-Standard+ X2; TC-MIDI X2; TC MIDI+ X2; TC-Double X2 & TC-Double+ X2
(Type Reference and Name) Sample Gas Cooler
4. **Name of Listing Company:** Bühler Technologies GmbH
5. **Address of Listing Company:** Harkortstrasse 29
Ratingen, D-40880
Germany
6. The examination and test results are recorded in confidential report number:

3062014 dated 4th October 2018
7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

CSA-C22.2 No. 213-15, CAN/CSA-C22.2 No. 61010-1:2012
8. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.
9. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.
10. **Equipment Ratings:**

TC-Standard Models:

Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous locations with an ambient temperature rating of 0°C of up to 50°C.

Certificate issued by:

J.E. Marquedant
VP, Manager, Electrical Systems

4 October 2018

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC, 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmapprovals.com www.fmapprovals.com

SCHEDULE



Canadian Certificate Of Conformity No: FM18CA0010X

TC-MIDI and TC-Double Models:

Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous (classified) locations with an ambient temperature rating of 0°C of up to 60°C.

11. The marking of the equipment shall include:

TC-Standard Models:

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

TC-MIDI and TC-Double Models:

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

12. **Description of Equipment:**

General - The TC-6 sample gas chillers are intended to cool and dry the sample gas before going into the gas analysers. Sample gases contain vapour which has to be withdrawn before it reaches the gas analyser. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a preset temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

Construction – The equipment is housed in a brushed stainless steel IP20 enclosure.

Ratings - TC-Standard operate at 24VDC, 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 50°C. and TC-MIDI and TC-Double Models operate at 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 60°C.

4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)

b = Gas cooler model: 1 or 2
d, = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
h = Peristaltic Pumps; 0, 1, 3
j & k = Moisture detector / Filter; 00, 01, 10, or 11
l = Status Outputs; 0 or 1
n = Delta T control; 0 or 1

4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
h = Peristaltic Pumps; 0, 2, or 4
j & k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, 22

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

SCHEDULE



Canadian Certificate Of Conformity No: FM18CA0010X

- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 22, 27, 32 & 37
- h = Peristaltic Pumps; 0, 2, 4
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = no value assigned.

4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI + X2(fitted with 1 heat exchangers)

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- e = Gas paths; 1 or 2
- f,g = Heat exchangers; 60, 61, 65, 66, 70, 75, 80 or 85
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20 21, or 22
- l,m = Status output; 00 or 10
- n,o = Delta T control; 00 or 10

4496 312 b2d1fghijklm00 Thermoelectric Cooler, TC-MIDI + X2(fitted with 2 heat exchangers)

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- f,g = Heat exchangers; 22, 27, 32, or 37
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, or 11
- l,m = Status output; 00 or 10

4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double X2

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 10, 15, 20, 25, 30, or 35
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double+ X2

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 22, 27, 32, or 37
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

SCHEDULE



Canadian Certificate Of Conformity No: FM18CA0010X

13. Specific Conditions of Use:

- 1. When installed as Class I Division 2 equipment, the thermoelectric cooler shall be mounted within a tool-secured IP54 enclosure.*

14. Test and Assessment Procedure and Conditions:

This Certificate has been issued in accordance with FM Approvals Canadian Certification Scheme.

15. Schedule Drawings

A copy of the technical documentation has been kept by FM Approvals.

16. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
4 th October 2018	Original Issue.

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

CERTIFICATE OF CONFORMITY

1. HAZARDOUS LOCATION ELECTRICAL EQUIPMENT PER CANADIAN REQUIREMENTS

2. Certificate No: FM18CA0010X
3. Equipment:
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2; TC-MIDI+ X2; TC-Double X2 & TC-Double+ X2 Sample Gas cooler
4. Name of Listing Company: Bühler Technologies GmbH
5. Address of Listing Company: Harkortstraße 29, Ratingen D-40880, Germany
6. The examination and test results are recorded in confidential report number:

3062014 dated 4th October 2018

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

CSA C22.2 No. 213:2021, CSA C22.2 No. 61010-1:2019

8. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.
9. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.
10. Equipment Ratings:

TC-Standard

Nonincendive for Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

TC-Midi & TC Double

Nonincendive for Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

Certificate issued by:



J.E. Marquedant
VP, Manager - Electrical Systems

9 October 2024

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC, One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

F 348 (Jul 24)



SCHEDULE

Canadian Certificate of Conformity No: FM18CA0010X

11. The marking of the equipment shall include:

TC-Standard

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

TC-Midi & TC Double

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

12. Description of Equipment:

General - The TC- Standard; TC-MIDI & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly). Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-MIDI X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-MIDI+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

Construction – The equipment is housed in a brushed stainless-steel IP20 enclosure.

Ratings - TC-Standard operate at 24VDC, 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 50°C. and TC-MIDI and TC-Double Models operate at 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 60°C.

See Annex for Model Codes

13. Specific Conditions of Use:

1. When installed as Class I Division 2 equipment, the thermoelectric cooler shall be mounted within a tool-secured IP54 enclosure which is capable of accepting one or more of the Class I Division 2 wiring methods per the Canadian Electric Code (CSA C22.1).

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

F 348 (Jul 24)



SCHEDULE

Canadian Certificate of Conformity No: FM18CA0010X

14. Test and Assessment Procedure and Conditions:

This Certificate has been issued in accordance with FM Approvals Canadian Certification Scheme.

15. Schedule Drawings

A copy of the technical documentation has been kept by FM Approvals.

16. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
4th October 2018	Original Issue.
9 October 2024	<u>Supplement 1:</u> Report Reference: RR242035 dated 9 October 2024. Description of the Change(s): 1. Addition of product variants due to changes to electronics 2. CSA C22.2 No. 213:2015 updated to CSA C22.2 No. 213:2021 3. CSA C22.2 No. 61010-1:2012 updated to CSA C22.2 No. 61010-1:2019

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

F 348 (Jul 24)



SCHEDULE

Canadian Certificate of Conformity No: FM18CA0010X

FM Approvals

ANNEX

4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
h = Condensate drain; 00, 10 or 30
j & k = Moisture detector/Filter; 00, 01, 10, or 11
l = Status Outputs; 00 or 10
n = Delta T control; 00 or 10

4496 211b2d1fg0000l0n0p TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchanger for H2/O2 applications)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1 or 2
f, g = Heat exchanger; 10, 15, 10 or 15
l = Status Outputs; 00 or 10
n = Delta T control; 00 or 10
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
h = Condensate drain; 0, 2, or 4
j & k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21, 22
l = Status Outputs; 0 or 1
n = Delta T control; 0 or 1

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

F 348 (Jul 24)



SCHEDULE

Canadian Certificate of Conformity No: FM18CA0010X

FM Approvals

4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 22, 27, 32 or 37
h = Condensate drain; 0, 2, 4
j & k = Moisture detector/Filter; 00, 01, 10, or 11
l = Signal Outputs; 0 or 1
n = no value assigned.

4496 311 b2defghijklmno TC-MIDI X2(fitted with 1 heat exchangers)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas path; 1 or 2
f,g = Heat exchangers; 10, 15, 20, 25, 30 or 35
h = Condensate drain; 0, 1 or 3
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector/Filter; 00, 01, 10 or 11
l,m = Signal output; 00 or 10
n,o = Delta T control; 00 or 10

4496 311 b2defg0000lmnop TC-MIDI X2 (fitted with 1 heat exchangers for H2/O2 applications)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas path; 1 or 2
f,g = Heat exchangers; 10, 15, 60, 65
l,m = Signal output; 00 or 10
n,o = Delta T control; 00 or 10
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmapprovals.com www.fmapprovals.com

F 348 (Jul 24)



SCHEDULE

Canadian Certificate of Conformity No: FM18CA0010X

FM Approvals

4496 312 b2d1fghijklm00 TC-MIDI + X2(fitted with 2 heat exchangers)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
f,g = Heat exchangers; 60, 65, 61, 66, 70, 75, 80 or 85
h = Condensate drain; 0, 2, or 4
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21 or 22
l,m = Signal outputs; 00 or 10
n, o = Delta T Control; 00 or 10

4496 611a2c1efghijkl000 TC-Double X2

Description of Equipment:

a = Gas cooler types 1 or 2
c = Voltage; 1 or 2
e,f = Heat exchangers; 10, 15, 20, 25, 30 or 35
g = Condensate drain; 0, 2, or 4
h = Sample gas pumps; 0, 1, or 2
i,j = Humidity sensor/Filter; 00, 01, 10, or 11
k,l = Signal outputs; 00 or 10

4496 611a2c1efghijkl000 TC-Double+ X2

Description of Equipment:

a = Gas cooler types 1 or 2
c = Voltage; 1 or 2
e,f = Heat exchangers; 22, 27, 32, or 37
g = Peristaltic pumps; 0, 2, or 4
h = Sample gas pumps; 0, 1, or 2
i,j = Moisture Detector/Filter; 00, 01, 10, or 11
k,l = Status output; 00 or 10

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

F 348 (Jul 24)



Page 6 of 6

CERTIFICATE OF CONFORMITY



1. **HAZARDOUS (CLASSIFIED) LOCATION ELECTRICAL EQUIPMENT PER US REQUIREMENTS**

2. **Certificate No:** FM18US0021X

3. **Equipment:** C-Standard X2; TC-Standard+ X2; TC-MIDI X2; TC MIDI+ X2;
(Type Reference and Name) TC-Double X2 & TC-Double+ X2

4. **Name of Listing Company:** **Sample Gas cooler**
Bühler Technologies GmbH

5. **Address of Listing Company:** **Harkortstrasse 29**
Ratingen, D-40880
Germany

6. The examination and test results are recorded in confidential report number:

3062014 dated 4th October 2018

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

FM Class 3600:2018, FM Class 3611:2018, FM Class 3810:2018,
ANSI/ISA-12.12.01-2015, ANSI/ISA 61010-1:2012

8. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

9. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.

10. Equipment Ratings:

TC-Standard Models:

Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous (classified) locations with an ambient temperature rating of 0°C to 50°C.

Certificate issued by:

J.E. Marquedant
VP, Manager, Electrical Systems

4 October 2018

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC, 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmapprovals.com www.fmapprovals.com

SCHEDULE



US Certificate Of Conformity No: FM18US0021X

TC-MIDI and TC-Double Models:

Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous (classified) locations with an ambient temperature rating of 0°C to 60°C.

11. The marking of the equipment shall include:

TC-Standard Models:

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

TC-MIDI and TC-Double Models:

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

12. **Description of Equipment:**

General - The TC- Standard; TC-Midi & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-Midi X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-Midi+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

Construction – The equipment is housed in a brushed stainless IP20 enclosure.

Ratings - TC-Standard operate at 24VDC, 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C up to 50°C. and TC-MIDI and TC-Double Models operate at 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C up to 60°C.

4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

SCHEDULE



US Certificate Of Conformity No: FM18US0021X

- b = Gas cooler model: 1 or 2
- d, = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 1, 3
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 2, or 4
- j & k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, 22
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 22, 27, 32 & 37
- h = Peristaltic Pumps; 0, 2, 4
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = no value assigned.

4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI + X2(fitted with 1 heat exchangers)

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- e = Gas paths; 1 or 2
- f,g = Heat exchangers; 60, 61, 65, 66, 70, 75, 80 or 85
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, or 22
- l,m = Status output; 00 or 10
- n,o = Delta T control; 00 or 10

4496 312 b2d1fghijklm00 Thermoelectric Cooler, TC-MIDI + X2(fitted with 2 heat exchangers)

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- f,g = Heat exchangers; 22, 27, 32, or 37
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, or 11
- l,m = Status output; 00 or 10

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

SCHEDULE



US Certificate Of Conformity No: FM18US0021X

4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double X2

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 10,15, 20,25,30, or 35
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double+ X2

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 22, 27, 32, or 37
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

13. Specific Conditions of Use:

1. *When installed as Class I Division 2 equipment, the thermoelectric cooler shall be mounted within a tool-secured IP54 enclosure which is capable of accepting one or more of the Class I Division 2 wiring methods per the National Electric Code (ANSI/NFPA 70).*

14. Test and Assessment Procedure and Conditions:

This Certificate has been issued in accordance with FM Approvals US Certification Requirements.

15. Schedule Drawings

A copy of the technical documentation has been kept by FM Approvals.

16. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
4 th October 2018	Original Issue.

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

CERTIFICATE OF CONFORMITY



1. **HAZARDOUS (CLASSIFIED) LOCATION ELECTRICAL EQUIPMENT PER US REQUIREMENTS**

2. **Certificate No:** FM18US0021X

3. **Equipment:** TC-Standard X2; TC-Standard+ X2; TC-MIDI X2; TC MIDI+ X2; TC-Double X2 & TC-Double+ X2

(Type Reference and Name)
Sample Gas cooler
4. **Name of Listing Company:** Bühler Technologies GmbH

5. **Address of Listing Company:** Harkortstrasse 29
Ratingen, D-40880
Germany

6. The examination and test results are recorded in confidential report number:

3062014 dated 4th October 2018

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

FM Class 3600:2018, FM Class 3611:2018, FM Class 3810:2018,
ANSI/ISA-12.12.01-2015, ANSI/ISA 61010-1:2012

8. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

9. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.

10. Equipment Ratings:

TC-Standard Models:

Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous (classified) locations with an ambient temperature rating of 0°C to 50°C.

Certificate issued by:

J.E. Marquedant
VP, Manager - Electrical Systems

25 January 2021

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

SCHEDULE



US Certificate Of Conformity No: FM18US0021X

TC-MIDI and TC-Double Models:

Non-incendive for Class I, Division 2, Groups A, B, C and D; T4 hazardous (classified) locations with an ambient temperature rating of 0°C to 60°C.

11. The marking of the equipment shall include:

TC-Standard Models:

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

TC-MIDI and TC-Double Models:

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

12. **Description of Equipment:**

General - The TC- Standard; TC-Midi & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-Midi X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-Midi+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

Construction – The equipment is housed in a brushed stainless IP20 enclosure.

Ratings - TC-Standard operate at 24VDC, 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 50°C. and TC-MIDI and TC-Double Models operate at 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 60°C.

4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

SCHEDULE



US Certificate Of Conformity No: FM18US0021X

- b = Gas cooler model: 1 or 2
- d, = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 1, 3
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
- h = Peristaltic Pumps; 0, 2, or 4
- j & k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, 22
- l = Status Outputs; 0 or 1
- n = Delta T control; 0 or 1

4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)

- b = Gas cooler model: 1 or 2
- d = Supply voltage; 1, 2 or 4
- f & g = Heat exchanger; 22, 27, 32 & 37
- h = Peristaltic Pumps; 0, 2, 4
- j & k = Moisture detector / Filter; 00, 01, 10, or 11
- l = Status Outputs; 0 or 1
- n = no value assigned.

4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI X2(fitted with 1 heat exchangers)

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- e = Gas paths; 1 or 2
- f,g = Heat exchangers; 60, 61, 65, 66, 70, 75, 80 or 85
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, or 22
- l,m = Status output; 00 or 10
- n,o = Delta T control; 00 or 10

4496 312 b2d1fghijklm00 Thermoelectric Cooler, TC-MIDI + X2(fitted with 2 heat exchangers)

- b = Gas cooler types 1 or 2
- d = Supply Voltage; 1 or 2
- f,g = Heat exchangers; 22, 27, 32, or 37
- h = Peristaltic pumps; 0, 2, or 4
- i = Sample gas pumps; 0, 1, 2, 6, or 7
- j,k = Moisture detector / Filter; 00, 01, 02, 10, or 11
- l,m = Status output; 00 or 10

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

SCHEDULE



US Certificate Of Conformity No: FM18US0021X

4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double X2

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 10, 15, 20, 25, 30, or 35
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

4496 611a2c1efghijkl000 Thermoelectric Cooler, TC-Double+ X2

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 22, 27, 32, or 37
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k,l = Status output; 00 or 10

13. Specific Conditions of Use:

1. *When installed as Class I Division 2 equipment, the thermoelectric cooler shall be mounted within a tool-secured IP54 enclosure which is capable of accepting one or more of the Class I Division 2 wiring methods per the National Electric Code (ANSI/NFPA 70).*

14. Test and Assessment Procedure and Conditions:

This Certificate has been issued in accordance with FM Approvals US Certification Requirements.

15. Schedule Drawings

A copy of the technical documentation has been kept by FM Approvals.

16. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
4 th October 2018	Original Issue.
25 th January 2021	Supplement 1: Report Reference: RR226270 dated 25 th January 2021. Description of the Change: Add digital interface and correct typo in model code to remove + for TC-MIDI fitted with 1 heat exchanger.

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

SCHEDULE



US Certificate Of Conformity No: FM18US0021X

FM Approvals

FM Approvals

FM Approvals

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. 1151 Boston-Providence Turnpike, Norwood, MA 02062 USA
T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

CERTIFICATE OF CONFORMITY

1. HAZARDOUS (CLASSIFIED) LOCATION ELECTRICAL EQUIPMENT PER US REQUIREMENTS

2. Certificate No: FM18US0021X
3. Equipment:
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2; TC-MIDI+ X2; TC-Double X2 & TC-Double+ X2
Sample Gas cooler
4. Name of Listing Company: Bühler Technologies GmbH
5. Address of Listing Company: Harkortstraße 29, Ratingen D-40880, Germany
6. The examination and test results are recorded in confidential report number:

3062014 dated 4th October 2018

7. FM Approvals LLC, certifies that the equipment described has been found to comply with the following Approval standards and other documents:

FM 3600:2022, FM 3611:2021, FM 3810:2021, ANSI/UL 61010-1:2019, ANSI/UL 121201:2021

8. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.
9. This certificate relates to the design, examination and testing of the products specified herein. The FM Approvals surveillance audit program has further determined that the manufacturing processes and quality control procedures in place are satisfactory to manufacture the product as examined, tested and Approved.
10. Equipment Ratings:

TC-Standard

Nonincendive for Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

TC-Midi & TC Double

Nonincendive for Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

Certificate issued by:



J.E. Marquedant
VP, Manager - Electrical Systems

9 October 2024

Date

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC, One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

F 347 (Jul 24)



SCHEDULE

US Certificate of Conformity No: FM18US0021X

11. The marking of the equipment shall include:

TC-Standard

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 50°C

TC-Midi & TC Double

Class I Division 2, Groups A, B, C, D; T4 Ta = 0°C to 60°C

12. Description of Equipment:

General - The TC- Standard; TC-MIDI & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly). Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-MIDI X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-MIDI+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

Construction – The equipment is housed in a brushed stainless-steel IP20 enclosure.

Ratings - TC-Standard operate at 24VDC, 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 50°C. and TC-MIDI and TC-Double Models operate at 115 VAC or 230 VAC, selectable by ordering, with an ambient temperature rating of 0°C of up to 60°C.

See Annex for Model Codes

13. Specific Conditions of Use:

1. When installed as Class I Division 2 equipment, the thermoelectric cooler shall be mounted within a tool-secured IP54 enclosure which is capable of accepting one or more of the Class I Division 2 wiring methods per the National Electric Code (ANSI/NFPA 70).

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

F 347 (Jul 24)



SCHEDULE

US Certificate of Conformity No: FM18US0021X

14. Test and Assessment Procedure and Conditions:

This Certificate has been issued in accordance with FM Approvals US Certification Requirements.

15. Schedule Drawings

A copy of the technical documentation has been kept by FM Approvals.

16. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
4 October 2018	Original Issue.
25 January 2021	<u>Supplement 1:</u> Report Reference: RR226270 dated 25 th January 2021. Description of the Change: Add digital interface and correct typo in model code to remove + for TC-MIDI fitted with 1 heat exchanger.
9 October 2024	<u>Supplement 2:</u> Report Reference: RR242035 dated 9 October 2024. Description of the Change(s): 1. Addition of product variants due to changes to electronics 2. FM3600 updated to latest edition (2022) 3. FM3611 updated to latest edition (2021) 4. FM3810 updated to latest edition (2021) 5. ANSI/UL 121201:2015 updated to ANSI/UL 121201:2021 6. ANSI/ISA 61010-1:2012 updated to ANSI/UL 61010-1:2019

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

F 347 (Jul 24)



SCHEDULE

US Certificate of Conformity No: FM18US0021X

FM Approvals

ANNEX

4496 211b2d11gh0jkl0n0pTC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchanger)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
h = Condensate drain; 00, 10 or 30
j & k = Moisture detector/Filter; 00, 01, 10, or 11
l = Status Outputs; 00 or 10
n = Delta T control; 00 or 10

4496 211b2d1fg0000l0n0p TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchanger for H2/O2 applications)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1 or 2
f, g = Heat exchanger; 10, 15, 10 or 15
l = Status Outputs; 00 or 10
n = Delta T control; 00 or 10
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
h = Condensate drain; 0, 2, or 4
j & k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21, 22
l = Status Outputs; 0 or 1
n = Delta T control; 0 or 1

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmapprovals.com www.fmapprovals.com

F 347 (Jul 24)



SCHEDULE

US Certificate of Conformity No: FM18US0021X

FM Approvals

4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 22, 27, 32 or 37
h = Condensate drain; 0, 2, 4
j & k = Moisture detector/Filter; 00, 01, 10, or 11
l = Signal Outputs; 0 or 1
n = no value assigned.

4496 311 b2defghijklmno TC-MIDI X2(fitted with 1 heat exchangers)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas path; 1 or 2
f,g = Heat exchangers; 10, 15, 20, 25, 30 or 35
h = Condensate drain; 0, 1 or 3
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector/Filter; 00, 01, 10 or 11
l,m = Signal output; 00 or 10
n,o = Delta T control; 00 or 10

4496 311 b2defg0000lmnop TC-MIDI X2 (fitted with 1 heat exchangers for H2/O2 applications)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas path; 1 or 2
f,g = Heat exchangers; 10, 15, 60, 65
l,m = Signal output; 00 or 10
n,o = Delta T control; 00 or 10
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

F 347 (Jul 24)



SCHEDULE

US Certificate of Conformity No: FM18US0021X

FM Approvals

4496 312 b2d1fghijklm00 TC-MIDI + X2(fitted with 2 heat exchangers)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
f,g = Heat exchangers; 60, 65, 61, 66, 70, 75, 80 or 85
h = Condensate drain; 0, 2, or 4
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21 or 22
l,m = Signal outputs; 00 or 10
n, o = Delta T Control; 00 or 10

4496 611a2c1efghijkl000 TC-Double X2

Description of Equipment:

a = Gas cooler types 1 or 2
c = Voltage; 1 or 2
e,f = Heat exchangers; 10, 15, 20, 25, 30 or 35
g = Condensate drain; 0, 2, or 4
h = Sample gas pumps; 0, 1, or 2
i,j = Humidity sensor/Filter; 00, 01, 10, or 11
k,l = Signal outputs; 00 or 10

4496 611a2c1efghijkl000 TC-Double+ X2

Description of Equipment:

a = Gas cooler types 1 or 2
c = Voltage; 1 or 2
e,f = Heat exchangers; 22, 27, 32, or 37
g = Peristaltic pumps; 0, 2, or 4
h = Sample gas pumps; 0, 1, or 2
i,j = Moisture Detector/Filter; 00, 01, 10, or 11
k,l = Status output; 00 or 10

To verify the availability of the Approved product, please refer to www.approvalguide.com

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals LLC. One Technology Way, Norwood, MA 02062 USA

T: +1 (1) 781 762 4300 F: +1 (1) 781 762 9375 E-mail: information@fmaprovals.com www.fmaprovals.com

F 347 (Jul 24)



1 TYPE EXAMINATION CERTIFICATE



2 Equipment or Protective systems intended for use in Potentially
Explosive Atmospheres - Directive 2014/34/EU

3 Type Examination Certificate No: FM18ATEX0012X

4 Equipment or protective system:
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2;
TC MIDI+ X2; TC-Double X2 & TC-Double+ X2
Sample Gas Cooler

5 Name of Applicant: Bühler Technologies GmbH

6 Address of Applicant: Harkortstrasse 29
Ratingen, D-40880
Germany

7 This equipment or protective system and any acceptable variation thereto is specified in the schedule to this certificate and documents therein referred to.

8 FM Approvals Europe Ltd. certifies that this equipment has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment intended for use in potentially explosive atmospheres given in Annex II to the Directive.

The examination and test results are recorded in confidential report number:

3062014 dated 04th October 2018

9 Compliance with the Essential Health and Safety Requirements, with the exception of those identified in item 15 of the schedule to this certificate, has been assessed by compliance with the following documents:

EN 60079-0:2012+A11:2013, EN 60079-7:2015+A1:2018 & EN 60079-15:2018

10 If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

11 This Type Examination certificate relates only to the design, examination and tests of the specified equipment or protective system in accordance to the Directive 2014/34/EU. Further requirements of the Directive apply to the manufacturing process and supply of this equipment or protective system. These are not covered by this certificate.

12 The marking of the equipment or protective system shall include:



II 3 G Ex ec nC IIC T4 Gc

Ta = 0°C to +40°C or 0°C to +50°C (TC-Standard X2 & TC-Standard+ X2 Models)

Ta = 0°C to +40°C or 0°C to +60°C (TC-MIDI X2 & TC-MIDI+ X2 and
TC-Double X2 & TC-Double+ X2 Models)


FM Approvals
Member of the FM Global Group

Digitally signed by Damien Mc Ardle
DN: cn=Damien Mc Ardle, o=FM
Approvals, ou=FM Approvals Europe
Ltd,
email=damien.mcardle@fmapproval
s.com, c=IE
Date: 2020.02.18 18:14:19 Z

Damien Mc Ardle
Certification Manager, FM Approvals Europe Ltd.

Issue date: 18th February 2020

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440
T: +353 (0) 1761 4200 E-mail: atex@fmapprovals.com www.fmapprovals.com

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

13 Description of Equipment or Protective System:

The TC- Standard; TC-Midi & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analysers. Sample gases contain vapour which has to be withdrawn before it reaches the gas analyser. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-Midi X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-Midi+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimise wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimise wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

TC-Standard X2 - Sample Gas Cooler (fitted with 1 or 2 heat exchangers)

Electrical data: Umax 24VDC, 115VAC or 230 VAC, 50/60 Hz, TC – Standard Models	130 W
TC – MIDI Models	290 W
TC – Double models	390 W

4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)

b	= Gas cooler model: 1 or 2
d,	= Supply voltage; 1, 2 or 4
f,g	= Heat exchanger; 10, 15, 20, 25, 30, or 35
h	= Peristaltic Pumps; 0, 1, 3
j,k	= Moisture detector / Filter; 00, 01, 10, or 11
l	= Status Outputs; 0 or 1
n	= Delta T control; 0 or 1

4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)

b	= Gas cooler model: 1 or 2
d	= Supply voltage; 1, 2 or 4
f,g	= Heat exchanger; 10, 15, 20, 25, 30, or 35
h	= Peristaltic Pumps; 0, 2, or 4
j,k	= Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, 22
l	= Status Outputs; 0 or 1
n	= Delta T control; 0 or 1

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

4496 212b2d2fgh0jkl000 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f,g = Heat exchanger; 22, 27, 32 or 37
h = Peristaltic Pumps; 0, 2, 4
j,k = Moisture detector / Filter; 00, 01, 10, or 11
l = Status Outputs; 0 or 1

4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI X2 (fitted with 1 gas path inside the heat exchanger)

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas paths; 1 or 2
f,g = Heat exchangers; 10, 15, 20, 25, 30, or 35
h = Peristaltic pumps; 0, 1, or 3
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector / Filter; 00, 01, 10, or 11
l,m = Status output; 00 or 10
n,o = Delta T control; 00 or 10

4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI X2 (fitted with 2 gas paths inside the heat exchanger)

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas paths; 1 or 2
f,g = Heat exchangers; 60, 61, 65, 66, 70, 75, 80 or 85
h = Peristaltic pumps; 0, 2, or 4
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, or 22
l,m = Status output; 00 or 10
n,o = Delta T control; 00 or 10

4496 312 b2d1fghijklmno Thermoelectric Cooler, TC-MIDI X2 (fitted with 2 heat exchangers)

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
f,g = Heat exchangers; 22, 27, 32, or 37
h = Peristaltic pumps; 0, 2, or 4
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector / Filter; 00, 01, 10, or 11
l,m = Status output; 00 or 10
n,o = Delta T control; 00 or 10

4496 312 b2d1fghijklm00 Thermoelectric Cooler, TC-MIDI + X2 (fitted with 2 heat exchangers in series)

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
f,g = Heat exchangers; 22, 27, 32, or 37
h = Peristaltic pumps; 0, 2, or 4
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector / Filter; 00, 01, 10, or 11
l,m = Status output; 00 or 10

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

4496 611a2c1efghijk000 Thermoelectric Cooler, TC-Double X2 (fitted with 2 heat exchangers in series)

- a = Gas cooler types 1, 2, 3 or 4
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 10,15, 20,25,30, or 35
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k = Status output; 0 or 1

4496 611a2c1efghijk000 Thermoelectric Cooler, TC-Double+ X2

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 22, 27, 32, or 37
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11

14 Specific Conditions of Use:

1. *The equipment shall be mounted in an enclosure providing a minimum degree of protection of IP54 in accordance with EN 60079-15, and in a tool-secured enclosure which meets the requirements of EN 60079-0 and EN 60079-15.*

15 Essential Health and Safety Requirements:

The relevant EHSRs that have not been addressed by the standards listed in this certificate have been identified and assessed in the confidential report identified in item 8.

16 Test and Assessment Procedure and Conditions:

This Type Examination Certificate is the result of testing of a sample of the product submitted, in accordance with the provisions of the relevant specific standard(s), and assessment of supporting documentation. It does not imply an assessment of the whole production.

Whilst this certificate may be used in support of a manufacturer's claim for CE Marking, FM Approvals Europe Ltd accepts no responsibility for the compliance of the equipment against all applicable Directives in all applications.

This Certificate has been issued in accordance with FM Approvals Europe Ltd's ATEX Certification Scheme.

17 Schedule Drawings

A list of the significant parts of the technical documentation is annexed to this certificate and a copy has been kept by FM Approvals Europe Ltd.

18 Certificate History

Details of the supplements to this certificate are described below:

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

Date	Description
15 th October 2018	Original Issue.
18 th February 2020	<u>Supplement 1:</u> Report Reference: RR222218 dated 17 th February 2020. Description of the Change: 1. A correction of typographical errors in model code section and the electrical power ratings. 2. Certificate transferred from FM Approvals Ltd., notified body no. 1725, to FM Approvals Europe Ltd., notified body no. 2809 3. Update CDL

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440
T: +353 (0) 1761 4200 E-mail: atex@fmaprovals.com www.fmaprovals.com



1 TYPE EXAMINATION CERTIFICATE

2 Equipment or Protective systems intended for use in Potentially
Explosive Atmospheres - Directive 2014/34/EU

3 Type Examination Certificate No: FM18ATEX0012X

4 Equipment or protective system:
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2;
TC MIDI+ X2; TC-Double X2 & TC-Double+ X2
Sample Gas Cooler

5 Name of Applicant: Bühler Technologies GmbH

6 Address of Applicant: Harkortstrasse 29
Ratingen, D-40880
Germany

7 This equipment or protective system and any acceptable variation thereto is specified in the schedule to this certificate and documents therein referred to.

8 FM Approvals Europe Ltd. certifies that this equipment has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment intended for use in potentially explosive atmospheres given in Annex II to the Directive.

The examination and test results are recorded in confidential report number:

3062014 dated 04th October 2018

9 Compliance with the Essential Health and Safety Requirements, with the exception of those identified in item 15 of the schedule to this certificate, has been assessed by compliance with the following documents:

EN 60079-0:2012+A11:2013, EN 60079-7:2015+A1:2018 and EN 60079-15:2018

10 If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

11 This Type Examination certificate relates only to the design, examination and tests of the specified equipment or protective system in accordance to the Directive 2014/34/EU. Further requirements of the Directive apply to the manufacturing process and supply of this equipment or protective system. These are not covered by this certificate.

12 The marking of the equipment or protective system shall include:



II 3 G Ex ec nC IIC T4 Gc

Ta = 0°C to +40°C or 0°C to +50°C (TC-Standard X2 & TC-Standard+ X2 Models)

Ta = 0°C to +40°C or 0°C to +60°C (TC-MIDI X2 & TC-MIDI+ X2 and
TC-Double X2 & TC-Double+ X2 Models)

Damien McArdle

Damien Mc Ardle
Certification Manager, FM Approvals Europe Ltd.

Issue date: 26th January 2021

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE



FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440
T: +353 (0) 1761 4200 E-mail: atex@fmaprovals.com www.fmaprovals.com

F ATEX 029 (Mar/2019)

Page 1 of 5

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

13 Description of Equipment or Protective System:

The TC- Standard; TC-Midi & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analysers. Sample gases contain vapour which has to be withdrawn before it reaches the gas analyser. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-Midi X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-Midi+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimise wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimise wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set to different temperatures.

TC-Standard X2 - Sample Gas Cooler (fitted with 1 or 2 heat exchangers)

Electrical data: Umax 24VDC, 115VAC or 230 VAC, 50/60 Hz, TC – Standard Models	130 W
TC – MIDI Models	290 W
TC – Double models	390 W

4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)

b	= Gas cooler model: 1 or 2
d,	= Supply voltage; 1, 2 or 4
f,g	= Heat exchanger; 10, 15, 20, 25, 30, or 35
h	= Peristaltic Pumps; 0, 1, 3
j,k	= Moisture detector / Filter; 00, 01, 10, or 11
l	= Status Outputs; 0 or 1
n	= Delta T control; 0 or 1

4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)

b	= Gas cooler model: 1 or 2
d	= Supply voltage; 1, 2 or 4
f,g	= Heat exchanger; 10, 15, 20, 25, 30, or 35
h	= Peristaltic Pumps; 0, 2, or 4
j,k	= Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, 22
l	= Status Outputs; 0 or 1
n	= Delta T control; 0 or 1

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

4496 212b2d2fgh0jkl000 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)

- b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f,g = Heat exchanger; 22, 27, 32 or 37
h = Peristaltic Pumps; 0, 2, 4
j,k = Moisture detector / Filter; 00, 01, 10, or 11
l = Status Outputs; 0 or 1

4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI X2 (fitted with 1 gas path inside the heat exchanger)

- b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas paths; 1 or 2
f,g = Heat exchangers; 10, 15, 20, 25, 30, or 35
h = Peristaltic pumps; 0, 1, or 3
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector / Filter; 00, 01, 10, or 11
l,m = Status output; 00 or 10
n,o = Delta T control; 00 or 10

4496 311 b2defghijklmno Thermoelectric Cooler, TC-MIDI + X2 (fitted with 2 gas paths inside the heat exchanger)

- b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas paths; 1 or 2
f,g = Heat exchangers; 60, 61, 65, 66, 70, 75, 80 or 85
h = Peristaltic pumps; 0, 2, or 4
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector / Filter; 00, 01, 02, 10, 11, 20, 21, or 22
l,m = Status output; 00 or 10
n,o = Delta T control; 00 or 10

4496 312 b2d1fghijklmno Thermoelectric Cooler, TC-MIDI X2 (fitted with 2 heat exchangers)

- b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
f,g = Heat exchangers; 22, 27, 32, or 37
h = Peristaltic pumps; 0, 2, or 4
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector / Filter; 00, 01, 10, or 11
l,m = Status output; 00 or 10
n,o = Delta T control; 00 or 10

4496 312 b2d1fghijklm00 Thermoelectric Cooler, TC-MIDI + X2 (fitted with 2 heat exchangers in series)

- b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
f,g = Heat exchangers; 22, 27, 32, or 37
h = Peristaltic pumps; 0, 2, or 4
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector / Filter; 00, 01, 10, or 11
l,m = Status output; 00 or 10

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

4496 611a2c1efghijk000 Thermoelectric Cooler, TC-Double X2 (fitted with 2 heat exchangers in series)

- a = Gas cooler types 1, 2, 3 or 4
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 10, 15, 20, 25, 30, or 35
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11
- k = Status output; 0 or 1

4496 611a2c1efghijk000 Thermoelectric Cooler, TC-Double+ X2

- a = Gas cooler types 1 or 2
- c = Voltage; 1 or 2
- e,f = Heat exchangers; 22, 27, 32, or 37
- g = Peristaltic pumps; 0, 2, or 4
- h = Sample gas pumps; 0, 1, or 2
- i,j = Moisture Detector/Filter; 00, 01, 10, or 11

14 Specific Conditions of Use:

1. *The equipment shall be mounted in an enclosure providing a minimum degree of protection of IP54 in accordance with EN 60079-15, and in a tool-secured enclosure which meets the requirements of EN 60079-0 and EN 60079-15.*

15 Essential Health and Safety Requirements:

The relevant EHSRs that have not been addressed by the standards listed in this certificate have been identified and assessed in the confidential report identified in item 8.

16 Test and Assessment Procedure and Conditions:

This Type Examination Certificate is the result of testing of a sample of the product submitted, in accordance with the provisions of the relevant specific standard(s), and assessment of supporting documentation. It does not imply an assessment of the whole production.

Whilst this certificate may be used in support of a manufacturer's claim for CE Marking, FM Approvals Europe Ltd accepts no responsibility for the compliance of the equipment against all applicable Directives in all applications.

This Certificate has been issued in accordance with FM Approvals Europe Ltd's ATEX Certification Scheme.

17 Schedule Drawings

A list of the significant parts of the technical documentation is annexed to this certificate and a copy has been kept by FM Approvals Europe Ltd.

18 Certificate History

Details of the supplements to this certificate are described below:

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

Date	Description
15 th October 2018	Original Issue.
18 th February 2020	<u>Supplement 1:</u> Report Reference: RR222218 dated 17 th February 2020. Description of the Change: 1. A correction of typographical errors in model code section and the electrical power ratings. 2. Certificate transferred from FM Approvals Ltd., notified body no. 1725, to FM Approvals Europe Ltd., notified body no. 2809 3. Update CDL
26 th January 2021	<u>Supplement 2:</u> Report Reference: RR226270 dated 25 th January 2021. Description of the Change: Add digital interface and correct typo in model code to remove + for TC-MIDI fitted with 1 heat exchanger.

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440
T: +353 (0) 1761 4200 E-mail: atex@fmaprovals.com www.fmaprovals.com



1. TYPE EXAMINATION CERTIFICATE

2. Equipment or Protective systems intended for use in Potentially Explosive Atmospheres - Directive 2014/34/EU

3. Type Examination Certificate No: FM18ATEX0012X

4. Equipment or protective system:
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2;
TC-MIDI+ X2; TC-Double X2 & TC-Double+ X2
Sample Gas Cooler

5. Name of Applicant: Bühler Technologies GmbH

6. Address of Applicant Harkortstraße 29, Ratingen D-40880, Germany

7. This equipment or protective system and any acceptable variation thereto is specified in the schedule to this certificate and documents therein referred to.

8. FM Approvals Europe Ltd, certifies that this component has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment intended for use in potentially explosive atmospheres given in Annex II to the Directive.

The examination and test results are recorded in confidential report number:

3062014 dated 4th October 2018

9. Compliance with the Essential Health and Safety Requirements, with the exception of those identified in item 15 of the schedule to this certificate, has been assessed by compliance with the following documents:

EN IEC 60079-0:2018, EN 60079-7:2015+A1:2018, EN IEC 60079-15:2019

10. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

11. This Type Examination certificate relates only to the design, examination and tests of the specified equipment or protective system in accordance to the Directive 2014/34/EU. Further requirements of the Directive apply to the manufacturing process and supply of this equipment or protective system. These are not covered by this certificate.

Certificate issued by:

Certification Manager, FM Approvals Europe Ltd.

Date 10 October 2024

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440
T: +353 (0) 1761 4200 E-mail: atex@fmapprovals.com www.fmapprovals.com

F ATEX 029 (Jul/2024)



Page 1 of 6

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

12. The marking of the equipment or protective system shall include:



TC-Standard

II 3 G Ex ec nC IIC T4 Gc

Ta = 0°C to +40°C or 0°C to +50°C

TC-MIDI & TC Double

II 3 G Ex ec nC IIC T4 Gc

Ta = 0°C to +40°C or 0°C to +60°C

13. **Description of Equipment or Protective System:**

The TC- Standard; TC-MIDI & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-MIDI X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-MIDI+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

TC-Standard X2 - Sample Gas Cooler (fitted with 1 or 2 heat exchangers)

Electrical data: Umax 24VDC, 115VAC or 230 VAC, 50/60 Hz

TC – Standard Models 130 W

TC – MIDI Models 290 W

TC – Double models 390 W

See Annex for Model Codes

14. **Specific Conditions of Use:**

1. The equipment shall be installed within a tool-secured enclosure providing a minimum degree of protection of IP54 and meeting the requirements of EN 60079-0 or certified as Ex e and in

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440

T: +353 (0) 1761 4200 E-mail: atex@fmapprovals.com www.fmapprovals.com

F ATEX 029 (Jul/2024)

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

compliance with the enclosure, mounting, spacing and segregation requirements of the ultimate application.

15. Essential Health and Safety Requirements:

The relevant EHSRs that have not been addressed by the standards listed in this certificate have been identified and assessed in the confidential report identified in item 8.

16. Test and Assessment Procedure and Conditions:

This Type Examination Certificate is the result of testing of a sample of the product submitted, in accordance with the provisions of the relevant specific standard(s), and assessment of supporting documentation. It does not imply an assessment of the whole production.

Whilst this certificate may be used in support of a manufacturer's claim for CE Marking, FM Approvals Europe Ltd accepts no responsibility for the compliance of the equipment against all applicable Directives in all applications.

This Certificate has been issued in accordance with FM Approvals Europe Ltd's ATEX Certification Scheme.

17. Schedule Drawings

A list of the significant parts of the technical documentation is annexed to this certificate and a copy has been kept by FM Approvals Europe Ltd.

18. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
15 October 2018	Original Issue.
18 February 2020	<u>Supplement 1:</u> Report Reference: RR222218 dated 17 th February 2020. Description of the Change: 1. A correction of typographical errors in model code section and the electrical power ratings. 2. Certificate transferred from FM Approvals Ltd., notified body no. 1725, to FM Approvals Europe Ltd., notified body no. 2809 3. Update CDL
26 January 2021	<u>Supplement 2:</u> Report Reference: RR226270 dated 25 th January 2021. Description of the Change: Add digital interface and correct typo in model code to remove + for TC-MIDI fitted with 1 heat exchanger.
10 October 2024	<u>Supplement 3:</u> Report Reference: RR242035 dated 9 October 2024. Description of the Change(s): 1. Addition of product variants due to changes to electronics 2. EN 60079-0:2012+A11:2013 updated to EN IEC 60079-0:2018

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

ANNEX

4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
h = Condensate drain; 00, 10 or 30
j & k = Moisture detector/Filter; 00, 01, 10, or 11
l = Status Outputs; 00 or 10
n = Delta T control; 00 or 10

4496 211b2d1fg0000l0n0p TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchanger for H2/O2 applications)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1 or 2
f, g = Heat exchanger; 10, 15, 10 or 15
l = Status Outputs; 00 or 10
n = Delta T control; 00 or 10
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
h = Condensate drain; 0, 2, or 4
j & k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21, 22
l = Status Outputs; 0 or 1
n = Delta T control; 0 or 1

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440
T: +353 (0) 1761 4200 E-mail: atex@fmapprovals.com www.fmapprovals.com

F ATEX 029 (Jul/2024)

4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 22, 27, 32 or 37
h = Condensate drain; 0, 2, 4
j & k = Moisture detector/Filter; 00, 01, 10, or 11
l = Signal Outputs; 0 or 1
n = no value assigned.

4496 311 b2defghijklmno TC-MIDI X2(fitted with 1 heat exchangers)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas path; 1 or 2
f,g = Heat exchangers; 10, 15, 20, 25, 30 or 35
h = Condensate drain; 0, 1 or 3
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector/Filter; 00, 01, 10 or 11
l,m = Signal output; 00 or 10
n,o = Delta T control; 00 or 10

4496 311 b2defg0000lmnop TC-MIDI X2 (fitted with 1 heat exchangers for H2/O2 applications)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas path; 1 or 2
f,g = Heat exchangers; 10, 15, 60, 65
l,m = Signal output; 00 or 10
n,o = Delta T control; 00 or 10
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

4496 312 b2d1fghijklm00 TC-MIDI + X2(fitted with 2 heat exchangers)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
f,g = Heat exchangers; 60, 65, 61, 66, 70, 75, 80 or 85
h = Condensate drain; 0, 2, or 4
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21 or 22
l,m = Signal outputs; 00 or 10
n, o = Delta T Control; 00 or 10

4496 611a2c1efghijkl000 TC-Double X2

Description of Equipment:

a = Gas cooler types 1 or 2
c = Voltage; 1 or 2
e,f = Heat exchangers; 10, 15, 20, 25, 30 or 35
g = Condensate drain; 0, 2, or 4
h = Sample gas pumps; 0, 1, or 2
i,j = Humidity sensor/Filter; 00, 01, 10, or 11
k,l = Signal outputs; 00 or 10

4496 611a2c1efghijkl000 TC-Double+ X2

Description of Equipment:

a = Gas cooler types 1 or 2
c = Voltage; 1 or 2
e,f = Heat exchangers; 22, 27, 32, or 37
g = Peristaltic pumps; 0, 2, or 4
h = Sample gas pumps; 0, 1, or 2
i,j = Moisture Detector/Filter; 00, 01, 10, or 11
k,l = Status output; 00 or 10

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE



1. TYPE EXAMINATION CERTIFICATE

2. Equipment or Protective systems intended for use in Potentially Explosive Atmospheres - Directive 2014/34/EU

3. Type Examination Certificate No: FM18ATEX0012X

4. Equipment or protective system:
(Type Reference and Name) TC-Standard X2; TC-Standard+ X2; TC-MIDI X2;
TC-MIDI+ X2; TC-Double X2 & TC-Double+ X2
Sample Gas Cooler

5. Name of Applicant: Bühler Technologies GmbH

6. Address of Applicant Harkortstraße 29, Ratingen D-40880, Germany

7. This equipment or protective system and any acceptable variation thereto is specified in the schedule to this certificate and documents therein referred to.

8. FM Approvals Europe Ltd, certifies that this component has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment intended for use in potentially explosive atmospheres given in Annex II to the Directive.

The examination and test results are recorded in confidential report number:

3062014 dated 4th October 2018

9. Compliance with the Essential Health and Safety Requirements, with the exception of those identified in item 15 of the schedule to this certificate, has been assessed by compliance with the following documents:

EN IEC 60079-0:2018, EN 60079-7:2015+A1:2018, EN IEC 60079-15:2019

10. If the sign 'X' is placed after the certificate number, it indicates that the equipment is subject to specific conditions of use specified in the schedule to this certificate.

11. This Type Examination certificate relates only to the design, examination and tests of the specified equipment or protective system in accordance to the Directive 2014/34/EU. Further requirements of the Directive apply to the manufacturing process and supply of this equipment or protective system. These are not covered by this certificate.

Certificate issued by:

FM Approvals

6 December 2024

Certification Manager, FM Approvals Europe Ltd.

Date

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

FM Approvals Europe Ltd. One Georges Quay Plaza, Dublin. Ireland. D02 E440
T: +353 (0) 1761 4200 E-mail: atex@fmapprovals.com www.fmapprovals.com
F ATEX 029 (Jul/2024)



12. The marking of the equipment or protective system shall include:



TC-Standard

II 3 G Ex ec nC IIC T4 Gc
Ta = 0°C to +40°C or 0°C to +50°C

TC-MIDI & TC Double

II 3 G Ex ec nC IIC T4 Gc
Ta = 0°C to +40°C or 0°C to +60°C

13. Description of Equipment or Protective System:

The TC- Standard; TC-MIDI & TC-Double sample gas chillers are intended to cool and dry the sample gas before going into the gas analyzers. Sample gases contain vapor which has to be withdrawn before it reaches the gas analyzer. The Gas flows through a heat exchanger (impinger) inserted into a cooling block. The latter then is cooled to a pre-set temperature (5°C mostly).

Depending on the required cooling capacity the size of the heat exchanger and therefore chiller is chosen and depending on the kind of gas to be cooled different heat exchanger materials are provided (stainless steel, glass or PVDF).

A gas cooler (chiller) might be prepared for more than one heat exchanger. The cooling block is cooled by different combinations of Peltier-elements. The temperature is sensed by an RTD.

The TC-Standard X2 / TC-MIDI X2 series of sample coolers are designed specifically for high cooling capacities and high ambient temperatures.

The TC-Standard+ X2 / TC-MIDI+ X2 series are designed specifically for the requirements in automated measuring systems (AMS) according to EN 15267-3. The series connection of the heat exchangers will cool in two cycles to minimize wash out effects.

The TC-Double X2 series are designed specifically for high cooling capacities, high ambient temperatures and to cool in two cycles to minimize wash out effects.

The TC-Double+ X2 incorporates two cooling blocks that can be set do different temperatures.

TC-Standard X2 - Sample Gas Cooler (fitted with 1 or 2 heat exchangers)

Electrical data: Umax 24VDC, 115VAC or 230 VAC, 50/60 Hz

TC – Standard Models 130 W

TC – MIDI Models 290 W

TC – Double models 390 W

See Annex for Model Codes

14. Specific Conditions of Use:

1. The equipment shall be installed within a tool-secured enclosure providing a minimum degree of protection of IP54 and meeting the requirements of EN 60079-0 or certified as Ex e and in

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

SCHEDULE

to Type Examination Certificate No. FM18ATEX0012X

compliance with the enclosure, mounting, spacing and segregation requirements of the ultimate application.

15. Essential Health and Safety Requirements:

The relevant EHSRs that have not been addressed by the standards listed in this certificate have been identified and assessed in the confidential report identified in item 8.

16. Test and Assessment Procedure and Conditions:

This Type Examination Certificate is the result of testing of a sample of the product submitted, in accordance with the provisions of the relevant specific standard(s), and assessment of supporting documentation. It does not imply an assessment of the whole production.

Whilst this certificate may be used in support of a manufacturer's claim for CE Marking, FM Approvals Europe Ltd accepts no responsibility for the compliance of the equipment against all applicable Directives in all applications.

This Certificate has been issued in accordance with FM Approvals Europe Ltd's ATEX Certification Scheme.

17. Schedule Drawings

A list of the significant parts of the technical documentation is annexed to this certificate and a copy has been kept by FM Approvals Europe Ltd.

18. Certificate History

Details of the supplements to this certificate are described below:

Date	Description
15 October 2018	Original Issue.
18 February 2020	<u>Supplement 1:</u> Report Reference: RR222218 dated 17 th February 2020. Description of the Change: 1. A correction of typographical errors in model code section and the electrical power ratings. 2. Certificate transferred from FM Approvals Ltd., notified body no. 1725, to FM Approvals Europe Ltd., notified body no. 2809 3. Update CDL
26 January 2021	<u>Supplement 2:</u> Report Reference: RR226270 dated 25 th January 2021. Description of the Change: Add digital interface and correct typo in model code to remove + for TC-MIDI fitted with 1 heat exchanger.

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

SCHEDULE
to Type Examination Certificate No. FM18ATEX0012X

Date	Description
10 October 2024	<u>Supplement 3:</u> Report Reference: RR242035 dated 10 October 2024. Description of the Change(s): 1. Addition of product variants due to changes to electronics 2. EN 60079-0:2012+A11:2013 updated to EN IEC 60079-0:2018
6 December 2024	<u>Supplement 4:</u> Report Reference: RR243713 dated 5 December 2024. Description of the Change(s): Document Updates

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

ANNEX

4496 211b2d1fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchangers)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
h = Condensate drain; 00, 10 or 30
j & k = Moisture detector/Filter; 00, 01, 10, or 11
l = Status Outputs; 00 or 10
n = Delta T control; 00 or 10

4496 211b2d1fg0000l0n0p TC-Standard X2 - Sample Gas Cooler (fitted with 1 heat exchanger for H2/O2 applications)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1 or 2
f, g = Heat exchanger; 10, 15, 10 or 15
l = Status Outputs; 00 or 10
n = Delta T control; 00 or 10
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

4496 212b2d2fgh0jkl0n0 TC-Standard X2 - Sample Gas Cooler (fitted with 2 heat exchangers)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 10, 15, 20, 25, 30, or 35
h = Condensate drain; 0, 2, or 4
j & k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21, 22
l = Status Outputs; 0 or 1
n = Delta T control; 0 or 1

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

4496 212b2d2fgh0jkl0n0 TC-Standard+ X2 - Sample Gas Cooler (with 2 heat exchangers in series)

Description of Equipment:

b = Gas cooler model: 1 or 2
d = Supply voltage; 1, 2 or 4
f & g = Heat exchanger; 22, 27, 32 or 37
h = Condensate drain; 0, 2, 4
j & k = Moisture detector/Filter; 00, 01, 10, or 11
l = Signal Outputs; 0 or 1
n = no value assigned.

4496 311 b2defghijklmno TC-MIDI X2(fitted with 1 heat exchangers)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas path; 1 or 2
f,g = Heat exchangers; 10, 15, 20, 25, 30 or 35
h = Condensate drain; 0, 1 or 3
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector/Filter; 00, 01, 10 or 11
l,m = Signal output; 00 or 10
n,o = Delta T control; 00 or 10

4496 311 b2defg0000lmnop TC-MIDI X2 (fitted with 1 heat exchangers for H2/O2 applications)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
e = Gas path; 1 or 2
f,g = Heat exchangers; 10, 15, 60, 65
l,m = Signal output; 00 or 10
n,o = Delta T control; 00 or 10
p = heat exchanger optimized for high-purity hydrogen/oxygen; -H2 or -O2

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

4496 312 b2d1fghijklm00 TC-MIDI + X2(fitted with 2 heat exchangers)

Description of Equipment:

b = Gas cooler types 1 or 2
d = Supply Voltage; 1 or 2
f,g = Heat exchangers; 60, 65, 61, 66, 70, 75, 80 or 85
h = Condensate drain; 0, 2, or 4
i = Sample gas pumps; 0, 1, 2, 6, or 7
j,k = Moisture detector/Filter; 00, 01, 02, 10, 11, 20, 21 or 22
l,m = Signal outputs; 00 or 10
n, o = Delta T Control; 00 or 10

4496 611a2c1efghijkl000 TC-Double X2

Description of Equipment:

a = Gas cooler types 1 or 2
c = Voltage; 1 or 2
e,f = Heat exchangers; 10, 15, 20, 25, 30 or 35
g = Condensate drain; 0, 2, or 4
h = Sample gas pumps; 0, 1, or 2
i,j = Humidity sensor/Filter; 00, 01, 10, or 11
k,l = Signal outputs; 00 or 10

4496 611a2c1efghijkl000 TC-Double+ X2

Description of Equipment:

a = Gas cooler types 1 or 2
c = Voltage; 1 or 2
e,f = Heat exchangers; 22, 27, 32, or 37
g = Peristaltic pumps; 0, 2, or 4
h = Sample gas pumps; 0, 1, or 2
i,j = Moisture Detector/Filter; 00, 01, 10, or 11
k,l = Status output; 00 or 10

THIS CERTIFICATE MAY ONLY BE REPRODUCED IN ITS ENTIRETY AND WITHOUT CHANGE

RMA-Formular und Erklärung über Dekontaminierung

Formulaire RMA et déclaration de décontamination



RMA-Nr./ Numéro de renvoi

Die RMA-Nr. bekommen Sie von Ihrem Ansprechpartner im Vertrieb oder Service. Bei Rücksendung eines Altgeräts zur Entsorgung tragen Sie bitte in das Feld der RMA-Nr. "WEEE" ein./ Le numéro d'autorisation de retour (RMA) est mis à votre disposition par votre interlocuteur à la vente ou au service. Lors du renvoi d'un appareil usagée en vue de sa mise au rebut, veuillez saisir "WEEE" dans le champ du n° RMA.

Zu diesem Rücksendeschein gehört eine Dekontaminierungserklärung. Die gesetzlichen Vorschriften schreiben vor, dass Sie uns diese Dekontaminierungserklärung ausgefüllt und unterschrieben zurücksenden müssen. Bitte füllen Sie auch diese im Sinne der Gesundheit unserer Mitarbeiter vollständig aus./ Une déclaration de décontamination fait partie intégrante de ce bulletin de retour. Les prescriptions légales vous obligent à nous renvoyer cette déclaration de décontamination remplie et signée. Veuillez la remplir également complètement au sens de la santé de nos employés.

Firma/ Société

Firma/ Société

Straße/ Rue

PLZ, Ort/ CP, localité

Land/ Pays

Gerät/ Appareil

Anzahl/ Nombre

Auftragsnr./ Numéro de commande

Ansprechpartner/ Interlocuteur

Name/ Nom

Abt./ Dépt.

Tel./ Tél.

E-Mail

Serien-Nr./ N° de série

Artikel-Nr./ N° d'article

Grund der Rücksendung/ Motif du retour

- ☐ Kalibrierung/ Calibrage ☐ Modifikation/ Modification
☐ Reklamation/ Réclamation ☐ Reparatur/ Réparation
☐ Elektroaltgerät/ Appareil électrique usagé (WEEE)
☐ andere/ autre

bitte spezifizieren/ veuillez spécifier

Ist das Gerät möglicherweise kontaminiert?/ L'appareil a-t-il été utilisé ?

- ☐ Nein, da das Gerät nicht mit gesundheitsschädlichen Stoffen betrieben wurde./ Non, car l'appareil n'a pas été utilisé avec des substances dangereuses pour la santé.
☐ Nein, da das Gerät ordnungsgemäß gereinigt und dekontaminiert wurde./ Non, car l'appareil a été nettoyé et décontaminé en bonne et due forme.
☐ Ja, kontaminiert mit:/ Oui, contaminé avec:



☐
explosiv/
explosif



☐
entzündlich/
inflammable



☐
brandfördernd/
comburant



☐
komprimierte
Gase/
gaz comprimés



☐
ätzend/
corrosif



☐
giftig,
Lebensgefahr/
toxique, danger
de mort



☐
gesundheitsge-
fährdend/
dangereux pour
la santé



☐
gesund-
heitsschädlich/
nocif pour la
santé



☐
umweltge-
fährdend/
dangereux pour
l'environnement

Bitte Sicherheitsdatenblatt beilegen! / Merci de joindre la fiche technique de sécurité

Das Gerät wurde gespült mit:/ L'appareil a été rincé avec:

Diese Erklärung wurde korrekt und vollständig ausgefüllt und von einer dazu befugten Person unterschrieben. Der Versand der (dekontaminierten) Geräte und Komponenten erfolgt gemäß den gesetzlichen Bestimmungen.

Falls die Ware nicht gereinigt, also kontaminiert bei uns eintrifft, muss die Firma Bühler sich vorbehalten, diese durch einen externen Dienstleister reinigen zu lassen und Ihnen dies in Rechnung zu stellen.

Firmenstempel/ Cachet de l'entreprise

Cette déclaration a été correctement complétée et signée par une personne autorisée. L'envoi des appareils et composants (décontaminés) se fait selon les conditions légales.

Si la marchandise nous est retournée sans avoir été nettoyée, donc toujours contaminée, la société Bühler se réserve le droit de faire nettoyer le produit par un prestataire externe et de vous envoyer la facture correspondante.

Datum/ Date

rechtsverbindliche Unterschrift/ Signature autorisée



Vermeiden von Veränderung und Beschädigung der einzusendenden Baugruppe

Die Analyse defekter Baugruppen ist ein wesentlicher Bestandteil der Qualitätssicherung der Firma Bühler Technologies GmbH. Um eine aussagekräftige Analyse zu gewährleisten muss die Ware möglichst unverändert untersucht werden. Es dürfen keine Veränderungen oder weitere Beschädigungen auftreten, die Ursachen verdecken oder eine Analyse unmöglich machen.

Umgang mit elektrostatisch sensiblen Baugruppen

Bei elektronischen Baugruppen kann es sich um elektrostatisch sensible Baugruppen handeln. Es ist darauf zu achten, diese Baugruppen ESD-gerecht zu behandeln. Nach Möglichkeit sollten die Baugruppen an einem ESD-gerechten Arbeitsplatz getauscht werden. Ist dies nicht möglich sollten ESD-gerechte Maßnahmen beim Austausch getroffen werden. Der Transport darf nur in ESD-gerechten Behältnissen durchgeführt werden. Die Verpackung der Baugruppen muss ESD-konform sein. Verwenden Sie nach Möglichkeit die Verpackung des Ersatzteils oder wählen Sie selber eine ESD-gerechte Verpackung.

Einbau von Ersatzteilen

Beachten Sie beim Einbau des Ersatzteils die gleichen Vorgaben wie oben beschrieben. Achten Sie auf die ordnungsgemäße Montage des Bauteils und aller Komponenten. Versetzen Sie vor der Inbetriebnahme die Verkabelung wieder in den ursprünglichen Zustand. Fragen Sie im Zweifel beim Hersteller nach weiteren Informationen.

Einsenden von Elektroaltgeräten zur Entsorgung

Wollen Sie ein von Bühler Technologies GmbH stammendes Elektroprodukt zur fachgerechten Entsorgung einsenden, dann tragen Sie bitte in das Feld der RMA-Nr. „WEEE“ ein. Legen Sie dem Altgerät die vollständig ausgefüllte Dekontaminierungserklärung für den Transport von außen sichtbar bei. Weitere Informationen zur Entsorgung von Elektroaltgeräten finden Sie auf der Webseite unseres Unternehmens.

Éviter la modification et la détérioration du module à expédier

L'analyse d'unités défectueuses est un élément essentiel de l'Assurance Qualité de la société Bühler Technologies GmbH. Pour garantir une analyse pertinente, la marchandise doit être si possible contrôlée en l'état. Aucune modification ne doit être réalisée ni autre dommage se produire car les causes pourraient alors être masquées ou toute analyse serait rendue impossible.

Manipulation des modules à sensibilité électrostatique

Dans le cas d'unités électroniques, il peut s'agir de composants sensibles aux charges électrostatiques. Les composants doivent être traités en respectant les directives en matière de décharges électrostatiques. Selon le cas, les composants devraient être remplacés à un poste de travail ESD. Si cela n'est pas possible, des mesures respectant les directives en matière de décharges électrostatiques devraient être prises lors du remplacement. Le transport ne doit être réalisé que dans des conditions respectant les directives en matière de décharges électrostatiques. Les emballages des composants doivent être en conformité avec les directives en matière de décharges électrostatiques. Utilisez selon le cas l'emballage de pièces de rechange ou choisissez vous-même un emballage en conformité avec les directives en matière de décharges électrostatiques.

Montage de pièces de rechange

Veillez lors de l'insertion d'une pièce de rechange à ce que les conditions décrites ci-dessus soient respectées. Veillez à ce que le montage du produit et de tous les composants soit fait de manière appropriée. Remettez tous les câbles dans leur état d'origine avant la mise en service du produit. En cas de doute, adressez-vous au fabricant du produit pour avoir plus d'informations.

Renvoi d'appareils électriques usagés en vue de leur mise au rebut

Si vous souhaitez expédier un produit électrique manufacturé par Bühler Technologies GmbH en vue de sa mise au rebut correcte, veuillez saisir "WEEE" dans le champ du n° RMA. Pour le transport, joignez à l'appareil usagé la déclaration de décontamination entièrement remplie et bien visible de l'extérieur. Vous trouverez davantage d'informations concernant la mise au rebut des appareils électriques usagés sur le site Internet de notre entreprise.

